

## GeoPT15 - MSAN, Ocean Floor Sediment

**Veranstalter:** International Association of Geoanalysts and Geostandards Newsletter - GeoPT15

**Ringversuchsmaterial:** MSAN, Ocean Floor Sediment

**RV geschlossen:** 2004 – 8

**Literatur:** Proficiency Testing Report GeoPT15 (Laborcode CRB = P38)

### Hauptelemente [MA%]

	CRB	RV	1sRV	Z-Score
Na <sub>2</sub> O	4,25	4,22	0,07	---
MgO	3,66	3,68	0,06	---
Al <sub>2</sub> O <sub>3</sub>	15,47	15,7	0,21	---
SiO <sub>2</sub>	54,15	54,73	0,6	---
P <sub>2</sub> O <sub>5</sub>	0,263	0,26	0,006	---
SO <sub>3</sub>	0,142	---	---	---
K <sub>2</sub> O	1,4	1,41	0,03	---
CaO	5,63	5,53	0,09	---
TiO <sub>2</sub>	1,12	1,11	0,02	---
Fe <sub>2</sub> O <sub>3</sub> tot	8,22	8,06	0,12	---
MnO	0,143	0,56	0,004	---
L.O.I.	4,49	---	---	---

### Spurenelemente [µg/g]

	CRB	RV	1sRV	Z-Score
As	5	7,3	0,4	---
Ba	286	273	9,4	---
Co	21	23,7	1,2	---
Cr	69	77,4	3,2	---
Cu	55	59,4	2,6	---
Ga	16	17,6	0,9	---
Nb	6	6,25	0,38	---
Ni	29	29	1,4	---
Pb	21	17,4	0,9	---
Rb	28	21,9	1,6	---
Sr	381	361,4	101,9	---
V	216	197,9	7,1	---
Zn	87	92,6	3,7	---
Zr	132	139,7	5,3	---

### Legende

**CRB:** Ergebnisse CRB – **RV:** Ergebnisse Ringversuch -- **1s-RV:** Standardabweichung Ringversuch

**Z-Score:** Differenz des Messwertes vom Mittelwert des Ringversuchs -- \* Wert nicht zertifiziert

# GEOPT15 - AN INTERNATIONAL PROFICIENCY TEST FOR ANALYTICAL GEOCHEMISTRY LABORATORIES - REPORT ON ROUND 15 / June 2004 (Ocean floor sediment MSAN)

**Philip J. Potts<sup>1\*</sup>, Michael Thompson<sup>2</sup>, Simon R.N. Chenery<sup>3</sup>, Peter C. Webb<sup>1</sup>  
and WANG Yimin<sup>4</sup>**

<sup>1</sup>Department of Earth Sciences, The Open University, Walton Hall, Milton Keynes, MK7 6AA, UK.

<sup>2</sup>Department of Chemistry, Birkbeck College, Gordon House, London, WC1H 0PP, UK.

<sup>3</sup>British Geological Survey, Keyworth, Nottingham, NG12 5GG, UK.

<sup>4</sup> National Research Centre for Geoanalysis, 26 Baiwanzhuang Road, Beijing 100037, PR China.

\*Corresponding author: e-mail p.j.potts@open.ac.uk

*Keywords: Proficiency testing, quality assurance, GeoPT, GeoPT15 round, MSAN, ocean floor sediment*

## **Abstract**

Results are presented for GeoPT15, round fifteen of the GeoPT international proficiency testing programme for analytical geochemistry laboratories. The sample distributed for this round was MSAN, an ocean floor sediment sample collected and prepared as a candidate reference material by the National Research Centre for Geoanalysis, Beijing, P.R. China. In this report, contributed data are listed, together with an assessment of assigned values, z-scores and charts showing both the distribution of contributed results and the overall performance of participating laboratories.

## **Introduction**

This fifteenth round of the international proficiency testing programme, GeoPT15, was conducted in a similar manner to earlier rounds. The programme is designed to be part of the routine quality assurance scheme of analytical geochemistry laboratories. The trial involves distributing a sample of established homogeneity to participating laboratories, which are required to analyse the sample using a well-characterised technique or techniques operated under routine analytical conditions. Results are then tabulated by the organisers and z-scores calculated by comparing each analysed result submitted

with the value assigned to be the best estimate of the true composition. These assigned values were estimated by robust statistical analysis of all the contributed data. By examining the magnitude of the z-score, participating laboratories can decide whether the quality of their data is satisfactory in relation to both their chosen fitness-for-purpose criterion and results submitted by all the other laboratories contributing to the round, and choose to take corrective action if this appears justified.

Full details of the programme have been included in reports of previous rounds, the current publication status of which is listed in Appendix 1. More specifically, the procedures followed in this round comply with the protocol published for conducting the GeoPT series of proficiency tests (see [www.geoanalyst.org](http://www.geoanalyst.org)). In this report, therefore, only the features of the present round are included and readers interested in further details are invited to review the GeoPT protocol and previously published reports.

**Steering Committee for Round 14:** M. Thompson (Chair), P.J. Potts (Secretary), S.R.N. Chenery, P.C. Webb and WANG Yimin.

**Sample:** The Ocean floor sediment sample (MSAN) used in GeoPT15 was collected and prepared as a candidate reference material by the National Research Centre for Geoanalysis, Beijing, P.R.China, under the direction of Prof WANG Yimin.

The sample was tested for homogeneity by selecting at random ten packets of the material that had been prepared for distribution. Duplicate test portions from each packet were analysed by WD-XRF at the OU. For the elements that were assigned values, homogeneity was considered to be satisfactory for use in the GeoPT15 round. An analysis of the homogeneity results with additional comments is listed in Appendix 2.

#### **Timetable for GeoPT14:**

Distribution of sample: March 2004.

Deadline for submission of analytical results: 15th May 2003.

Distribution of draft report: June 2004

#### **Submission of results**

Results submitted by the seventy-nine laboratories that participated in this round are listed in Table 1. All these data (except P79 - late submission) were used for the assessment of assigned values.

#### **Assigned values**

Following procedures described in earlier rounds, a robust statistical procedure was used to derive assigned concentration values [ $X_a$ ], these being judged to be the best estimates of the true composition of this sample. Data in Table 2 lists assigned values for 10 major and 43 trace elements. Values were assigned on the basis that:

- (i) sufficient laboratories had contributed data for an element,
- (ii) the statistical assessment gave confidence that the results showed a central portion approximating to a normal distribution. Part of this assessment involved examining a bar chart for each element to judge the distribution of results. Bar charts for elements/species shown in Figure 1 were judged to have satisfactory distributions, namely:

SiO<sub>2</sub>, TiO<sub>2</sub>, Al<sub>2</sub>O<sub>3</sub>, Fe<sub>2</sub>O<sub>3</sub>T, MnO, MgO, CaO, Na<sub>2</sub>O, K<sub>2</sub>O, P<sub>2</sub>O<sub>5</sub>, As, Ba, Be, Br, Cd, Ce, Co, Cr, Cs, Cu, Dy, Er, Eu, Ga, Gd, Hf, Ho, La, Li, Lu, Mo, Nb, Nd, Ni, Pb,

Pr, Rb, Sb, Sc, Sm, Sn, Sr, Ta, Tb, Th, Tl, Tm, U, W, Y, Yb, Zn and Zr.

Of these, the elements As, Br, Cd, Sb and Sn were assigned provisional values, principally because data distributions plotted in Figure 1 possess some degree of asymmetry.

Charts in Figure 2 show distribution data for elements that were not judged to be sufficiently satisfactory in the statistical analysis to assign values. In the present round, values could not be assigned to the following elements/species, despite the availability of sufficient analytical results:

FeO, H<sub>2</sub>O<sup>+</sup>, CO<sub>2</sub>, LOI, B, Bi, Cl, F, Ge, Hg, I, S, Se, W. Of these, the element/species FeO, CO<sub>2</sub>, LOI and W are presented in Figure 2 with guidance values. There is some degree of consensus in results reported for these elements to provide some guidance to contributing laboratories. However, these data must be interpreted with caution.

For other elements that are not included in either of these two lists, insufficient data were reported to allow any assessment to be made.

The most common reasons for elements failing the assessment of assigned values were as follows:

- (i) Insufficient number of contributed results.
- (ii) Results showing a strong positive skew in the frequency distribution diagram, sometimes with an indication of multi-modality.
- (iii) A robust mean clearly different from the mode, which makes the determination of a consensus impracticable.
- (iv) A very wide distribution of results as judged by the robust standard deviation value so that no matter where the consensus was placed, most of the participants would receive an 'unsatisfactory' classification if z-scores were calculated.

#### **Z-score analysis**

As in previous rounds, laboratories were invited to choose one of two performance standards against which their analytical results would be judged:

**Data quality 1** for laboratories working to a 'pure geochemistry' standard of performance, where analytical results are designed for geochemical research and where care is taken to provide data of high precision and accuracy, sometimes at the expense of a reduced sample throughput rate.

**Data quality 2** for laboratories working to an 'applied geochemistry' standard of performance, where, although precision and accuracy are still important, the main objective is to provide results on large numbers of samples collected, for example, as part of geochemical mapping projects or geochemical exploration programmes.

The target standard deviation ( $H_a$ ) for each element assessed was calculated from a modified form of the Horwitz function as follows:

$$H_a = k \cdot X_a^{0.8495}$$

Where  $X_a$  is the concentration of the element expressed as a *fraction*, and the factor  $k = 0.01$  for pure geochemistry labs and  $k=0.02$  for applied geochemistry labs.

Z-scores were calculated for each elemental result submitted by each laboratory from:

$$z = [X - X_a] / H_a$$

where

$X$  is the contributed result,  $X_a$  is the assigned value and  $H_a$  is the target standard deviation.

Z-score results are listed in Table 3 and participating laboratories are invited to assess their performance using the following criterion:

Z-score results in the range  $-2 < z < 2$  are considered to be 'satisfactory' (in the sense that no action is called for by the participant). If the z-score for any element falls outside this range, contributing laboratories are advised to examine their procedures to ensure that determinations are not subject to unsuspected analytical bias.

### Overall performance

A summary of the overall performance of individual laboratories in this round is plotted in Figure 3 as a multiple z-score chart. In this chart, the z-score performance for each element is distinguished by symbols that make it simple to identify whether the

results were satisfactory or gave z-scores that exceeded the action limits. This chart is designed to help individual laboratories to judge their overall performance in this proficiency testing round.

### Participation in future rounds

The benefit from proficiency testing arises from regular participation and laboratories are invited to contribute to the GeoPT16 round, the sample for which will be distributed during September 2004.

### Acknowledgments

The authors thank Jann Matela and Liz Lomas (OU) for valued assistance with the production of this report. The GeoPT programme is organised on behalf of the International Association of Geoanalysts.

## Appendix 1

### Publication status of proficiency testing reports

---

#### GeoPT1

Thompson M., Potts P.J., Kane J.S. and Webb P.C. (1996)

GeoPT1. International proficiency test for analytical geochemistry laboratories - Report on round 1. *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis*, 20, 295-325.

#### GeoPT2

Thompson M., Potts P.J., Kane J.S., Webb P.C. and Watson, J.S. (1998)

GeoPT2. International proficiency test for analytical geochemistry laboratories - Report on round 2. *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis*, 22 127-156.

#### GeoPT3

Thompson M., Potts P.J., Kane J.S. and Chappell B.W. (1999a)

GeoPT3. International proficiency test for analytical geochemistry laboratories - Report on round 3. *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis*, 23, 87-121.

#### GeoPT4

Thompson M., Potts P.J., Kane J.S., Webb P.C. and Watson J.S. (1999b)

GeoPT4. International proficiency test for analytical geochemistry laboratories - Report on round 4. Published in the electronic version of *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis* (Summer 2000).

#### GeoPT5

Thompson M., Potts P.J., Kane J.S., and Wilson S. (1999c)

GeoPT5. International proficiency test for analytical geochemistry laboratories - Report on round 5. Published in the electronic version of *Geostandards Newsletter: The Journal of Geostandards and Geoanalysis* (Summer 2000).

#### GeoPT6

Potts P.J., Thompson M., Kane J.S., Webb P.C. and Carignan J. (2000)

GEOPT6 - an international proficiency test for analytical geochemistry laboratories - report on round 6 (OU-3: Nanhoron microgranite) and 6A (CAL-S: CRPG limestone). International Association of Geoanalysts: Unpublished report.

#### GeoPT7

Potts P.J., Thompson M., Kane J.S., and Petrov L.L. (2000)

GEOPT7 - an international proficiency test for analytical geochemistry laboratories - report on round 7 (GBPG-1

Garnet-biotite plagiogneiss). International Association of Geoanalysts: Unpublished report.

#### GeoPT8

Potts P.J., Thompson M., Kane J.S., Webb, P.C. and Watson J.S. (2000)

GEOPT8 - an international proficiency test for analytical geochemistry laboratories - report on round 8 / February 2001 (OU-4 Penmaenmawr microdiorite). International Association of Geoanalysts: Unpublished report.

#### GeoPT9

Potts P.J., Thompson M., Webb, P.C. and Watson J.S. (2001)

GEOPT9 - an international proficiency test for analytical geochemistry laboratories - report on round 9 / July 2001 (OU-6 Penrhyn slate). International Association of Geoanalysts: Unpublished report.

#### GeoPT10

Potts P.J., Thompson M., Webb, P.C., Watson J.S. and Wang Yimin (2001)

GEOPT10 - an international proficiency test for analytical geochemistry laboratories - report on round 10 / December 2001 (CH-1 Marine sediment). International Association of Geoanalysts: Unpublished report.

#### GeoPT11

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and Watson J.S. (2002)

GEOPT11 - an international proficiency test for analytical geochemistry laboratories - report on round 11 / July 2002 (OU-5 Leaton dolerite). International Association of Geoanalysts: Unpublished report.

#### GeoPT12

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and Batjargal B. (2003)

GEOPT12 - an international proficiency test for analytical geochemistry laboratories - report on round 12 / January 2003 (GAS Serpentinite). International Association of Geoanalysts: Unpublished report.

#### GeoPT13

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and Kaspar H.U. (2003)

GEOPT13 - an international proficiency test for analytical geochemistry laboratories - report on round 13 / July 2003 (Köln Loess). International Association of Geoanalysts: Unpublished report.

#### GeoPT14

Potts P.J., Thompson M., S.R. Chenery, Webb, P.C. and B. Batjarga (2004)

GeoPT14 - an international proficiency test for analytical geochemistry laboratories - report on round 14 / January 2004 (OShBO - alkaline granite). International Association of Geoanalysts: Unpublished report.

---

## Appendix 2 - GeoPT15 Homogeneity Report

The sample was tested for homogeneity by selecting at random ten packets of the material that had been prepared for distribution. Duplicate test portions from each packet were analysed by WD-XRF at the OU. Data for each element were carefully examined for features that would invalidate or unduly weaken the test for sufficient homogeneity. Elements for which the homogeneity data were thus inadequate were excluded from the analysis. The valid data sets were subjected element by element to one-way analysis of variance to derive a number of statistical parameters from which homogeneity could be assessed. Because of deficiencies in conventional homogeneity testing statistics, that can flag the presence of heterogeneity at a level that is statistically significant but inconsequential for the purposes of the proficiency test, overall conclusions were evaluated against a standard of 'sufficient homogeneity' as evaluated from the Fearn-Thompson test. The test refers to a different null hypothesis, namely  $H : \sigma_{sam}^2 \leq \sigma_{all}^2$ , where  $\sigma_{all}^2$  is the 'allowable' variance, the highest between-sample variance compatible with the nature of the proficiency test. In the GeoPT programme, conclusions from the Fearn-Thompson test are taken as definitive (T Fearn and M Thompson, *Analyst*, 2001, 126, 1414-1417).

Results from an evaluation of the homogeneity testing data obtained by the XRF analysis of both glass disks (for majors) and powder pellets (for traces) is given in the following two tables, in which only the key parameters are listed. As part of the data evaluation, it was noted that one Cochran outlier was detected in the major element results, but was eliminated, as allowed under the revised Harmonised Protocol. In addition, a slight trend was detected in the trace element data, and for some elements, the analytical precision was worse than the ideal limit (elements denoted by an '\*' in the table below). These discrepancies were judged not to invalidate the Fearn-Thompson statistic nor the overall conclusions of sufficient homogeneity.

Analyte	Concentration (% m/m)	Analytical variance	Sampling variance	Fearn statistic Critical level	Outcome
SiO <sub>2</sub>	54.6824	0.007812	0.006634	0.071268	OK
TiO <sub>2</sub>	1.0812	0.0000151	0.0000084	0.0000965	OK
Al <sub>2</sub> O <sub>3</sub>	15.7416	0.0005092	0.000329	0.00811	OK
Fe <sub>2</sub> O <sub>3</sub>	7.9675	0.000045	0.0000366	0.002422	OK
MnO	0.1558	0.0000011	0	0.0000042	OK
MgO	3.6584	0.0001009	0.000045	0.000745	OK
CaO	5.4593	0.0002036	0	0.001475	OK
Na <sub>2</sub> O	4.3421	0.0003511	0	0.001237	OK
K <sub>2</sub> O	1.3926	0.0000116	0	0.000135	OK
P <sub>2</sub> O <sub>5</sub>	0.2544	0.000004*	0.0000014	0.0000113	OK
LOI	4.5578	0.0006778*	0.000212	0.001674	OK

Analyte	Concentration ( $\mu\text{g g}^{-1}$ )	Analytical variance	Sampling variance	Critical level	Outcome
Rb	33.08	0.154	0.02475	0.568	OK
Sr	359.615	2.046	1.18008	25.876	OK
Y	28.585	0.101	0.02343	0.425	OK
Zr	144.073	0.522	1.29704	5.56	OK
Nb	6.278	0.116*	0	0.142	OK
Ba	255.625	119.403*	0	133.952	OK
Pb	16.848	0.875*	0.08971	1.015	OK
Th	3.472	0.154*	0.12603	0.164	OK
U	1.952	0.622*	0	0.632	OK
Sc	24.197	1.792*	1.26565	2.053	OK
V	202.25	41.339*	0	50.716	OK
Cr	76.59	4.485*	0	6.251	OK
Co	21.093	0.771*	0.40779	0.972	OK
Ni	30.018	0.602*	0.23285	0.959	OK
Cu	54.813	1.175*	0	2.161	OK
Zn	91.287	1.128	1.35778	3.458	OK
Ga	16.143	0.271*	0	0.396	OK
As	10.618	3.308*	0	3.402	OK

\*Exceeds the ideal limit.



GeoPT15 Table 1 concentration data

Round identifier	P1	P2	P3	P4	P5	P5	P6	P7	P7	P8	P8	P9	P9	P10	P10	P10	P11	P12	P12	P13	P13	P14	P14	P15	P15	P16	P16	P17	P17	P18	P18	P19	P19	P20	P20	P21	P21	P22	P22		
Hg	mg kg-1																																								
Ho	mg kg-1	1.02			1.03									1.14															0.98	0.918					1.014						
I	mg kg-1						54																																		
In	mg kg-1	0.07																																							
Ir	mg kg-1																																								
La	mg kg-1	17			17.5		17							16.6															16.6	14.19					16.24	19.9	12				
Li	mg kg-1	20.1																																							
Lu	mg kg-1	0.39			0.43									0.36															0.38	0.385					0.413						
Mo	mg kg-1	1.2					3																					1.1													
N	mg kg-1																																								
Nb	mg kg-1	5.7			6.7		4	6				8								5.9	7	8	6	6			6.1	6.22					6.693	7.3	105						
Nd	mg kg-1	22.8			21.7		17				17	18.8								17	28	37	26.4	31	31		21.7	18.82					21.69	20.8	16						
Ni	mg kg-1	30			44.7	28						29								17	28	37	26.4	31	31		31					37	29.63	26.5	33						
Os	mg kg-1																																								
Pb	mg kg-1				7.89	19.5		36	17.1			20								12	17	16	15.8	17							17.27	20	17.88	15.2	429						
Pd	mg kg-1																																								
Pr	mg kg-1	5.04			4.75		4																					5	4.289						5.121						
Pt	mg kg-1																																								
Rb	mg kg-1	33.8			32.1		30	32.4				36								34	33.7	38	29.8	34			40	35.58													
Re	mg kg-1																																								
Rh	mg kg-1																																								
Ru	mg kg-1																																								
S	mg kg-1						908		1137	1720																															
Sb	mg kg-1	0.51			0.89									0.47														0.3										1305			
Sc	mg kg-1								20.3					24.2														22.8	30.5												
Se	mg kg-1																																								
Sm	mg kg-1	5.13			4.85									4.92														5.1	4.325												
Sn	mg kg-1				5.1																							1.7													
Sr	mg kg-1	386			391		345	357.6																				1.7													
Ta	mg kg-1	0.42			0.45																							0.4	0.39												
Tb	mg kg-1	0.85			0.81									0.87														0.78	0.716												
Te	mg kg-1																																								
Th	mg kg-1	4.1			3.7																																				
Tl	mg kg-1																																								
Tl	mg kg-1																																								
Tm	mg kg-1	0.43			0.42																																				
U	mg kg-1	1.38			1.47																																				
V	mg kg-1	236			235																																				
W	mg kg-1	1.2			0.78																																				
Y	mg kg-1	26.8			26.3		24	28.9																																	
Yb	mg kg-1	2.8			2.96																																				
Zn	mg kg-1	93			102.7	122																																			
Zr	mg kg-1	132.5	135				110	133	143																																

Technique codes: A=ICP-AES; AA=AAS; C=colorimetry; E=(atomic) emission spectrometry; G=gravimetric; I=INAA; IR= infra red detection; ISE=ion selective electrodes; M=ICP-MS; O=other; S=spectrophotometry; T=titrimetry; W=wet chemistry; X=X-ray fluorescence. \*Results P79 were submitted too late to contribute to the assessment of assigned values.



GeoPT15 Table 1 concentration data

Round	P23	P24	P25	P26	P27	P28	P28	P28	P29	P30	P31	P32	P33	P34	P35	P36	P37	P37	P38	P39	P40	P41	P42	P43	P44	P45	P46
Sample	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN
Techniq	M, X	M	X	AA, ISE	AA, ISE	TX	TX	A, M	A, M	AAA, A, M, X	M, X	M, X	M, X	AAA, A, A, M, X	AO	I	I	X	A, I, R	I	M	AA, X	AA, X	AA, X	AA, X	MSAN	
Test poi	0.1-5	0.1	1.0-10	0.5-10	0.5	0.15-6	6	0.25	0.2-1	0.1-8	0.2-12	0.056	0.1-0.8	0.1-2	0.5	0.2	0.2	0.4-5	0.2-7	0.04	0.1	0.1-1	0.174	0.04-0	0.4	1.0-20	
Data qu	2	2	2	2	1	1	2	2	2	2	1	1	1	1	2	2	1	2	2	2	1	2	1	1	2	1	
SiO2	53.8		54.69	54		55.17		55.58	54.8	54.8	54.07		54.6	54.65	55.25		54.15	55.28		64.41	54.54	54.40	55	54.49			
TiO2	1.14		1.112	0.98	1.1	1.091		1.14	1.13	1.108	1.09		1.11	1.11	1.11	1.14		1.12	1.144		1.07	1.09	1.15	1.11	1.1		
Al2O3	15.84		15.98	15.34	16.9	15.82		16.06	15.8	15.46	15.54		15.75	16.06	14.61	16.61		15.47	15.78		27.76	15.58	16.10	15.77	15.76		
Fe2O3	8.14		8.123	8.08	7.6	8.132		7.924	8.35	8.098	7.92		8	8.21	8.25	7.96		8.22	8.13		4.69	8.38	8.20	8.09	8.12		
Fe(II)						3.35			3.43					2.995													
MnO	0.16		0.151	0.15	0.17	0.158		0.162	0.155	0.151	0.16		0.16	0.16	0.13	0.159		0.143	0.154		0.11	0.158	0.13	0.16	0.16		
MgO	3.6		3.659	3.49	3.8	3.751		3.667	3.65	3.529	3.6		3.66	3.77	4.03	4		3.66	3.609		3.9	3.8	3.77	3.77	3.61		
CaO	5.59		5.566	5.5	5.8	5.533		5.385	5.37	5.403	5.47		5.52	5.82	5.49	5.44		5.63	5.441		1.6	5.55	5.64	5.47	5.47		
Na2O	3.88		4.162	3.86	4.2	4.275		4.361	4.27	4.165	4.18		4.09	4.19	3.31	4.37		4.25	4.431		4.98	3.75	4.10	4.21	4.17		
K2O	1.47		1.42	1.36	1.2	1.435		1.5	1.43	1.444	1.37		1.37	1.45	1.39	1.44		1.4	1.399		4.56	1.32	1.20	1.45	1.36		
P2O5	0.27		0.268	0.28	0.25	0.267		0.268	0.259	0.238	0.26		0.28	0.27					0.263	0.269			0.241	0.25	0.26	0.27	
H2O+			1.35										3.83														
CO2									1.62				1.8	0.25					1.529								
LOI	5.7		4.712	4.77		4.59			4.89	5.61	4.77		5.07	4.325	6.1			4.49	4.51				5.54	5.12		4.47	
Ag																											
As	8		9.6	6.6					7	6.1	6.786			7.04	8	6.91		3	4.47	4.8						4	
Au																											
B																											
Ba	261	258.9			275	265.7		271.2	272	244	286.4	273	272	273		270		296	284	275	272.8						
Be					12			1.3	1.1	1.056	1.27	1.3	1.3														
Bi									0.11	0.8	1.9																
Br										67	73		75.3														
Cd									0.2	0.9	0.441		0.193	0.22													
Ce	35.32		44.4					32.05	34.9	40.4	35.2	33.9	36.27	34.7		36.7											
Cl								10490						11490		12900		10600	11998								
Co	22		24.9	36				21.85	23.5	26	22.35	22.7	24.57	21.8		22.7		21	25	25.2		17					
Cr	75		83.8	68.4		78.8		75.9	78	85	72.8	74.5	76.27	72		89.1		49	78.2	73.8							
Cs								1.53	1.72		1.793	1.86	1.5	1.7		1.6											
Cu	56		60	70.7	61	58.5		60.8	61	56	57	56.7	61.93	60.2		55		55	69.1							58	
Dy			4.972					4.61	5.2	5.4	4.875	4.74	4.71	5.08		5.43			5.05								
Er			2.917					2.81	2.95	3.2	2.931	2.69	2.73	3.02		2.94			2.94								
Eu			1.467					1.49	1.45	1.5	1.265	1.39	1.54	1.45		1.54			1.47								
F			354					300					314														
Ga	15		16	14.9				16.51	17.5	17	18.4	17.64	17.9	17		16			19.1							18	
Gd			5.071					4.54	5.15		5.141	4.79	5.35	5.08		5.44			5.44								
Ge								1.2	0.9				1.7						1.41								
Hf	4		3.44					3.58	3.6	2.4	3.907	3.04	3.72	4		3.89			3.52								

GeoPT15 Table 1 concentration data

Round	P23	P24	P24	P25	P26	P27	P28	P28	P29	P30	P31	P32	P33	P34	P35	P36	P37	P37	P38	P39	P40	P41	P42	P43	P44	P45	P46
Hg						0.022				0.02	0.04	0.02	0.019	21													
Ho	1.015								1.05	0.97	0.97	1.009	1.02	0.997	1.06				49	1.02		1.003					
I										0.06					0.06												
In																											
Ir																											
La	16.84		14.6				17	11.6	16	19	16.11	16.1	16.47	16.5						17.3	15.2	15.71					
Li						20			19.1		18.61		21.4	21													
Lu	0.419							0.39	0.4	0.47	0.409	0.37	0.431	0.45						0.45	0.45	0.405					
Mo								0.78	1.3	1.4	1.423		1.43							1.35						3	
N																											
Nb	5	6.98	2.4	6.5			5.8	5.26	6.7	5.4	6	5.84		6					6	5.76		6.33				8	
Nd	21.29							19.83	21	21.1	21.43	20.91	21.83	20.5						23.1	21	20.58					
Ni					32	25.6	27	29.3	25.6	29	26.7	28.3	29.6	30.9	25.2				29	27.8			25.7			30	
Os																											
Pb	15	18.5			20.4	16.5	22	17.8		17	17	16.8	15.2	16.43	18.4				21	17.4		17.37				20	
Pd																											
Pt	4.955							4.24	4.9	5.6	4.724	4.81	4.63	4.91					4.8			4.696					
Rb	31	33.58			32.2	30.8	33	29.69	31	29	30.4	31.4	33.33	33					28	32.6	35.4	31.51				35	
Re																											
Rh																											
Ru																											
S										1520				1630	0.15				1420	1646							
Sb									0.42		0.397			392	0.4					0.44	0.56						
Sc					27.8		30	24	24	27.5	21.8	24	24.97	23			24.5		19.5	25						18	
Se										0.4	1.1		0.584														
Sm	4.96							4.7	4.9	5	5.009	5.02	5.49	4.9					4.92	4.38	4.77						
Sn	3							1.32	1.3	1.7	1.412			1.5					2.09								
Sr	343	376.3			355.4	361	380	359.4	376.1	375	331	355.3	361	369	366				380			359.6				369	
Ta								0.41	0.62	1	0.403	0.4	0.463						0.27			0.383					
Tb								0.75	0.82	0.85	0.789	0.8	0.804	0.85					0.89	0.84	0.76						
Te										3				0.22													
Th	4	3.622			0	6.5		3	3.24	3.35	4	3.904	3.31	3.47	3.8				3.11	3.5	3.498					5	
Ti									0.27	1	0.203	0.31	0.267	0.29					0.26								
Tm		0.409						0.41	0.4	0.44	0.402	0.41	0.419	0.44					0.39			0.397					
U	3	1.499			0	3		2	1.31	1.4	2.6	1.646	1.33	1.42	1.5				1.53			1.31					
V	188				187.8	140	215	208.1	190	198	199	192.3	204	207.3	208				216	216							
W									1	2	0.996								0.79								
Y	26	27.71			27.4	27.5	29.8	30.2	25.8	27	28.3	28.81	29	27.1					26			29.06				31	
Yb		2.733						2.68	2.7	2.9	2.786	2.59	2.68	2.8					2.93	2.85	2.552						
Zn	84				92.2	81.3	105	92.5	99.6	95	88	92	96.6	88					99.4							94	
Zr	136		138	146.6	138	135	142.6	142.9	140	131	143.3	116	145.3	130					146	132	146					146	

GeoPT15 Table 1 concentration data

Round	P46	P47	P48	P49	P50	P51	P52	P52	P53	P54	P55	P56	P57	P58	P59	P60	P61	P62	P63	P64	P65	P66	P67	P68	P69	
Sample	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	
Techniq	X	M,X	A	A,O	A,AA	AAA	AAA	AAA	M,X	X	X	AA,IR	A,IR	X	X	A,X	M,X	A,M,X	A,AA	X	J,IR	O,X	A,AA	A,AA	A,AA	
Test poi	20	0.05-40.05-0.003-5	0.003-5	0.2-3	0.1-5	0.1-5	0.1-5	0.1-10	0.1-10	1.5	5	0.1-1	0.2-4	5	1	9	1-1.5	0.2-3.5	0.2-1	0.06-5	1	0.1-1.4	0.05-4	0.1	1.0-3	0.1-5
Data qu	2	2	2	2	1	2	2	2	1	2	2	2	2	2	1	2	2	1	2	1	1	1	2	2	2	
SiO2	55.1	54.54	55.48	53.83	54.71				54.95	54.31		54.8	54.02	58.69	54.92	55	54.25	56.1	53.568	53			54.55	55.2	54.09	
TiO2	1.16	1.101	1.124	1.04	1.11	1.121			1.096	1.1		1.09	1.13	1.05	1.094	1.1	1.086	1.1	1.097	1.13			1.23	1.14	1.127	
Al2O3	15.8	15.63	15.86	15.58	15.82	15.8			15.78	15.41		15.7	15.94	14.23	15.71	15.75	15.7	15.4	15.437	15	15.88	15.69	15.48	15.8	15.78	
Fe2O3	7.98	7.973	8.12	7.89	8.12	8.08			8.03	7.62		8	8.2	7.53	8.09	8.02	8.498	7.78	9.744	7.5	7.56	8.16	8.1	8.3	7.898	
Fe(II)									3.2	2.99	2.83	3.88	3.19						3.509							
MnO	0.141	0.158	0.155	0.166	0.15				0.156	0.154	0.158	0.16	0.16	0.14	0.153	0.16	0.156	0.16	0.153	0.14	0.16	0.15		0.166	0.16	0.153
MgO	3.79	3.654	3.53	3.51	3.86				3.685	3.76	3.63	3.64	3.66	2.69	3.87	3.88	3.808	3.03	3.889	3.7	3.64		3.64	3.6	3.588	
CaO	5.56	5.5	5.66	5.78	5.31	5.508			5.55	5.573	5.5	5.51	5.89	4.03	5.51	5.55	5.573	5.5	5.687	5.5	5.54		5.49	5.6	5.569	
Na2O	4.24	4.164	4.34	4.21	4.14	1.35			4.22	4.12		4.27	4.38	3.43	4.26	4.36	4.272	4.19	3.810	5.5	4.33	4.3		4.25	3.9	4.211
K2O	1.5	1.352	1.47	1.34	1.42	1.416			1.38	1.37		1.38	1.43	1.29	1.42	1.43	1.425	1.46	1.342	1.4	1.21	1.42		1.4	1.43	1.388
P2O5	0.267	0.261	0.26	0.23	0.26				0.255	0.277	0.268	0.26	0.25	0.17	0.26	0.26	0.265	0.26	0.251	0.22		0.25			0.25	0.266
H2O+									3.76	2.94		3.76	2.94													
CO2									1.55	1.49		1.55	1.49						0.332		1.83			1.5	1.674	
LOI	4.37								4.57	5.68	6.67	4.74				4.49	4.827	4.94	4.890	7.14	4.37		4.73	4.48	6.06	
Ag									0.196	0.14													0.24			
As									9.9	6.9						6		7.29					6.93			
Au																					7.4					
B																					0.003					
Ba	281	352	272.2	272	245				296	262		265	269.7			248	200	278.6	260	293	277	266		54.9	45.53	
Be									2.5	1.22			1.21						2.0					281	272.1	
Bi									0.11															1.12	1.2	
Br																								0.1	0.1	
Cd									0.26	0.19			0.098											93.6	100	
Ce	37	34.9							33.8			33.31					33.88	36.1	29.6				0.19			
Cl	26230																							30.9	36.25	
Co	31								29.08	24.4		23	22.11											11600	9700	
Cr	58	84							89	78.7		90	86.25			55	78.58	75.3	72.6	72	75			24.2	26.3	
Cr																								71.4	80.92	
Cs																								1.55	1.6	
Cu									73	60.3		58	57.62											59.9	59.48	
Dy									4.92	4.73		4.73												4.5	3.8	
Er									2.91	2.822		2.822												2.78	2	
Eu									1.51	1.376		1.376												1.49	1.3	
F																										
Ga									17.8	17.2		17	17.2											17	19.24	
Gd									5.12	4.933		4.933												4.71	4.2	
Ge	5.19								1.19																	
Ge																										
Hf									3.48	3.5		5	3.6											3.7	3.26	
Hf																									2.6	

GeoPT15 Table 1 concentration data

Round	P46	P47	P48	P49	P50	P51	P52	P52	P53	P54	P55	P56	P57	P58	P59	P59	P60	P61	P62	P63	P64	P65	P66	P66	P67	P68	P69
Hg					0.022		0.061																0.028				
Ho	0.98		0.925	0.84			1.07		1.02			0.958					1.079	1.05	0.84					0.94		0.7	
I																										4	
In																								0.061			
Ir																											
La	16	16.4		16.95	14		17.95		16.1			15.51				17.14	16.6	16.6			16.43		14.2	19.13	13		
Li			16.2	17.5	16.7	13.4	18		20.6			20.14				19.4	28.0						17.7	20.05	23	11	
Lr	0.4		0.37	0.38			0.42		0.4			0.393				0.416	0.42	0.31			0.44		0.39		0.3		
Mo							2.31	1.48				1.66											1.51		1.6		
N																											
Nb	7.43		6.5	6			7.54	6.92		8	9	6.1			6.8	6.381	5.08	8.3					6.02		10		
Nd	20.5		17.7	19.5			22.6		21.1			20.56				19.97	22.3	18.2			20		19.3		18.6		
Ni			29	25.2	12.5		38.8	29		33	27	29.33			36.8	25	29.9	31	36.6	28			29.2	31.82	26	27	
Os																											
Pb	15.48		18.4	22.7			16.4	17.8		19	13	17.9			20.9	17.27	16.3	18.2					16.9		26		
Pd																											
Pr	4.82		4.73	5.6			5.35		4.82			4.706				4.534	5.15	4.2					4.33		4		
Pt																											
Rb	32.57		33	29.2	32		26		32.8		34	32	32.2		39.5	34.26	31.7	37.2	37	33.4			36.4		29.8		
Re																											
Rh																											
Ru																											
S	1380			1198	700				1500	1280												1824				1060	0.099
Sb							3.1	0.41																			
Sc			23	21.1			43	24.4		13	23	22.78				25.98	22.9	29	24	23.4			0.55		0.4		
Se	3.11																										
Sm	5.05		4.09	5.4			5.51		5.14			4.69				5.203	5.47	4.52			5.08		4.64		4.4		
Sn							2.33	1.63		2.5		1.42					1.12	1.43					1.6		1.6		
Sr	381.3	228.7	362	345	340		385	360		382	368	360.7			336	396.5	352	400					340	362.5	313	340	
Ta							0.77	0.35				0.46				0.456		0.5			0.48		0.32		1		
Tb	0.81		0.77				0.81	0.83				0.76				0.859	0.84	0.65			0.82		0.73		0.6		
Te																											
Th	3.75			5.5			3.29		3.57		3	3.54				3.248	3.29	2.37			3.8		3.22		3		
Tl							0.26	0.29				0.29															
Tm	0.41		0.375	0.4			0.45		0.43			0.408				0.422	0.44	0.32					0.23		0.3		
U							1.44		1.38		2	1.462				1.364	1.28	0.96			1.5		1.23		1.5		
V	169	166	202	194	202	164	264	202		196	198.1				210	175	193.1	203	212	182			194	200.2	160	190	
W							2.86	0.52				0.68						0.47					0.72		1.4		
Y	27.29		27	24.2			29.52		28.2		30	26	25.76		25	35.12	27.3	28.5	24				25.1	29.71	16.8	24	
Yb	2.7		2.36	2.76			3		2.73			2.69				2.684	2.91	2.38			224		2.7		1.8		
Zn			95.1	93	84.7	90	106		93.4		93	91	81.96		86	78.64	75.2	98.7					93.9	103.9	97	89	
Zr	153	129.2	140	139	43		140	143.5		152	146	140.4			145	118.7	145	142	126				151	161.1	105	120	

GeoPT15 Table 1 concentration data

Round	P70	P71	P72	P73	P74	P74	P75	P76	P77	P78	P79*
Sample MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN
Techniq	A,M,X	X	M	IR,M	X	X	X	M	I	X	A,M
Test poi	1.0-6	0.2-0.5	0.6	0.25	0.04-7.4	7.5	5	0.1	0.1	0.1-0.2	0.2
Data qu	2	1	1	1	1	2	2	1	2	1	2
SiO2	54.95	55.84		54.41		54.3				55.12	54.15
TiO2	0.126	1.083		1.124		1.12				1.121	1.02
Al2O3	16.2	15.72		15.81		15				15.87	16.07
Fe2O3	8.11	7.854		8.15		9.55			7.935	8.192	7.8
Fe(II)				4.47							
MnO	0.154	0.151		0.156		0.149		0.15		0.166	0.15
MgO	3.65	3.595		3.66						3.705	3.57
CaO	5.5	5.56		5.57						5.599	5.35
Na2O	4.38	4.233		4.28						4.254	4.31
K2O	1.4	1.392		1.38		1.25				1.4	1.43
P2O5	0.271	0.264		0.269						0.275	0.27
H2O+				3.43							
CO2				1.5							
LOI	5.44	4.58		4.82							5.73
Ag											
As	9										
Alu										8.5	6.99
B											
Ba	297			263	278			277		259	2.62
Be								1.17		1.2	1.14
Bi								0.11		0.1	
Br	66										
Cd	7										
Ce	33			32.2	29.9			0.32		0.16	0.81
Cl						4520		35.2		30	33.9
Co	18			22.6	22			23.2	22.25		22
Cr	67				87			76.9		84	80.6
Cs				2.03				1.72	1.75	1.5	1.5
Cu	54			58.3	61			58.3		70	60.4
Dy				5.21	4.27			4.86		4.84	4.58
Er				2.97	2.49			2.97		2.94	2.6
Eu				1.54	1.41			1.47	1.45	1.58	1.42
F											
Ga	16			26.1	18			18.6		18.1	18.7
Gd				5.03	4.49			4.59		5.04	4.73
Ge								1.87		1.1	1.48
Hf	6			3.58	3.32			3.58	3.49	3.3	3.55

GeoPT15 Table 1 concentration data

Round	P70	P71	P72	P73	P74	P74	P75	P76	P77	P78	P79*
Hg											
Ho			0.932	0.91				1.02		1	0.914
I											
In											
Ir											
La	17		15.1	14.4				18.7	16.45	15.69	16
Li								19.4			
Lu			0.459	0.37				0.423	0.365	0.42	0.415
Mo	3							1.45		1.6	1.57
N				273							
Nb	9		5.76	5.59				5.92		6.3	5.47
Nd			19.8	18.5				21.6	17.2	20.12	20.5
Ni	25			32				29.6		30	30.5
Os											
Pb	17			17.1				18.1		19	18.1
Pd											
Pr			4.46	4.26				4.97		4.64	4.75
Pt											
Rb	33		28.4	31				31.5	34.7	33	30.9
Re											
Rh											
Ru											
S				1380						1400	
Sb								0.49		2	0.45
Sc				18.8				26.2	23.5	25	
Se											
Sm			4.72	4.57				4.91	4.815	5.42	4.81
Sn										1	4.38
Sr	345		351	362				364		376	349
Ta			0.478	0.33				0.44		0.1	0.44
Tb			0.936	0.71				0.769	0.79		0.757
Te											
Th			3.34	3.2				3.52	3.535	4.4	3.51
Ti								0.282			
Tm			0.406	0.38				0.421			0.395
U			1.4	1.22				1.46	1.4	1.5	1.44
V	129		189	197						197	191
W								0.94			0.76
Y	29		24.8	25.7				27.1		34.6	26.9
Yb			2.64	2.5				2.82	2.85	2.97	2.66
Zn	86			92				101		99	96.5
Zr	155		128	137				140		135	137

**Table 2 GeoPT 15 (MSAN - Ocean floor sediment)**

**Assigned values and robust statistical analysis of contributed data**

	$X_a$ % m/m	$H_a$ % m/m	sdm % m/m	sdm/ $H_a$	status		$X_a$ mg/kg	$H_a$ mg/kg	sdm mg/kg	sdm/ $H_a$	status
SiO2	54.73	0.60	0.08	0.13	assigned	La	16.3	0.9	0.2	0.2	assigned
TiO2	1.11	0.02	0.00	0.14	assigned	Li	19.2	1.0	0.5	0.5	assigned
Al2O3	15.70	0.21	0.03	0.16	assigned	Lu	0.406	0.037	0.006	0.161	assigned
Fe2O3T	8.06	0.12	0.02	0.21	assigned	Mo	1.47	0.11	0.05	0.45	assigned
MnO	0.156	0.004	0.001	0.198	assigned	Nb	6.26	0.38	0.11	0.29	assigned
MgO	3.68	0.06	0.02	0.25	assigned	Nd	20.2	1.0	0.3	0.3	assigned
CaO	5.53	0.09	0.01	0.17	assigned	Ni	29.0	1.4	0.5	0.3	assigned
Na2O	4.22	0.07	0.02	0.30	assigned	Pb	17.4	0.9	0.2	0.3	assigned
K2O	1.41	0.03	0.01	0.32	assigned	Pt	4.76	0.30	0.07	0.24	assigned
P2O5	0.260	0.006	0.002	0.248	assigned	Rb	32.9	1.6	0.4	0.2	assigned
As	7.3	0.4	0.3	0.7	provisional	Sb	0.49	0.04	0.03	0.67	provisional
Ba	272.6	9.4	2.5	0.3	assigned	Sc	23.8	1.2	0.3	0.2	assigned
Be	1.2	0.1	0.0	0.4	assigned	Sm	4.97	0.31	0.06	0.20	assigned
Br	72.0	3.0	2.2	0.7	provisional	Sn	1.6	0.1	0.1	0.8	provisional
Cd	0.19	0.02	0.01	0.60	provisional	Sr	361.8	11.9	2.4	0.2	assigned
Ce	34.4	1.6	0.4	0.3	assigned	Ta	0.424	0.039	0.022	0.569	assigned
Co	23.7	1.2	0.4	0.3	assigned	Tb	0.805	0.067	0.010	0.150	assigned
Cr	77.4	3.2	1.3	0.4	assigned	Th	3.51	0.23	0.06	0.25	assigned
Cs	1.66	0.12	0.03	0.22	assigned	Tl	0.27	0.03	0.01	0.38	assigned
Cu	59.4	2.6	0.7	0.3	assigned	Tm	0.409	0.037	0.005	0.120	assigned
Dy	4.84	0.31	0.07	0.24	assigned	U	1.42	0.11	0.02	0.18	assigned
Er	2.84	0.19	0.04	0.20	assigned	V	197.9	7.1	2.1	0.3	assigned
Eu	1.43	0.11	0.02	0.20	assigned	Y	27.2	1.3	0.4	0.3	assigned
Ga	17.6	0.9	0.3	0.3	assigned	Yb	2.76	0.19	0.03	0.16	assigned
Gd	5.01	0.31	0.08	0.25	assigned	Zn	92.6	3.7	1.0	0.3	assigned
Hf	3.57	0.24	0.06	0.25	assigned	Zr	139.7	5.3	1.3	0.3	assigned
Ho	0.992	0.080	0.010	0.131	assigned						

$X_a$  = assigned value calculated as the robust mean of submitted data.

$H_a$  = target precision calculated using a modified version of the Horwitz equation

for Data quality 1 ( $H_a = 0.01 X_a^{0.6665}$ )

sdm = standard deviation of the mean calculated from submitted data using robust statistics.

Table 3 GeoPT15																				
Z-score data for Ocean Floor Sediment MSAN																				
SUBMITTED DATA May 2004																				
Round identifier	P1	P2	P3	P4	P5	P5	P6	P7	P7	P8	P9	p9	P10	p10	P11	P12	P13	P14	P15	P16
Sample	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN
Technique codes	M.X	X	X	AA.X	M	M	X	X	X	IR.X	X	X	I	I	X	X	X	IR.O.X	IR.T.X	V.X
Test portion (g)	0.2-0.25	0.1	0.6	0.6-1	0.1	0.1	0.7-2	0.7-10	10	0.7-1	0.6-6	0.6-6	10-10	10	1.0-2	10	0.6-4	0.01-0.7	0.1-2	0.5-7
Date quality	2	2	1	2	1	2	2	1	2	2	1	2	1	2	2	2	1	1	2	2
SiO2	-0.4	*	-0.1	0.5	*	*	-0.6	0.2	*	0.3	-2.0	*	*	*	3.3	*	0.5	0.0	-0.2	0.3
TiO2	-1.1	*	-0.4	0.0	*	*	-4.4	-1.3	*	0.7	-0.9	*	*	*	1.4	-0.2	0.2	5.1	-0.2	0.2
Al2O3	0.7	*	-0.5	-2.2	*	*	-7.2	0.7	*	0.1	-1.2	*	*	*	-1.2	*	0.5	0.1	-0.1	-0.1
Fe2O3T	-0.6	*	-0.4	0.8	*	*	-1.7	-0.7	*	1.8	-2.0	*	*	*	-0.9	2.9	-0.9	1.9	-0.2	-0.1
Fe(II)O	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
MnO	*	*	-2.6	0.5	*	*	2.2	0.3	*	1.0	-1.4	*	*	*	0.3	0.5	0.7	1.0	0.0	-1.2
MgO	0.7	*	-0.2	-0.9	*	*	34.5	-0.5	*	0.9	0.9	*	*	*	10.2	*	2.4	-6.5	-0.6	-0.8
CaO	-0.3	*	-0.5	0.3	*	*	0.6	-0.7	*	0.9	-1.5	*	*	*	-2.3	4.5	-0.8	1.2	-2.9	0.5
Na2O	-0.3	*	2.2	0.1	*	*	*	2.0	*	-1.8	-0.9	*	*	*	0.2	2.9	*	-1.9	0.4	-0.1
K2O	-0.9	*	-1.5	2.1	*	*	11.2	-0.5	*	4.6	-3.7	*	*	*	2.4	0.8	3.2	-0.5	-1.1	0.0
P2O5	0.0	*	0.0	-3.2	*	*	*	-0.8	*	0.8	1.5	*	*	*	-4.3	*	-3.8	0.0	0.8	0.7
H2O+	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
CO2	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
LOI	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ag	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
As	*	0.0	*	1.7	*	*	*	*	7.2	*	*	0.2	*	-0.1	*	*	1.6	3.9	*	*
Au	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
B	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ba	*	*	*	*	0.1	*	1.2	*	-2.3	*	5.6	*	*	-0.8	0.8	*	-2.4	0.6	0.1	0.3
Be	*	-0.6	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Bi	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Br	*	*	*	*	*	*	-0.3	*	*	*	*	-0.2	*	0.3	*	1.5	*	*	*	*
Cd	*	-0.3	*	*	*	*	45.7	*	*	*	*	*	*	*	*	*	*	-9.8	*	*
Ce	*	-0.2	*	-0.3	*	*	0.8	*	*	*	*	-2.0	0.0	*	*	*	*	15.2	*	*
Cl	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Co	*	-0.2	*	*	1.9	*	*	*	-2.1	*	1.1	*	*	-0.2	*	*	0.2	4.6	-1.3	0.1
Cr	*	*	*	-3.6	4.6	*	9.4	*	-0.9	*	1.4	*	*	0.5	*	-1.2	6.1	8.6	-1.0	0.1
Cs	0.6	-0.6	*	*	*	*	*	*	*	*	*	*	*	0.6	*	*	*	-13.5	*	*
Cu	-1.1	*	*	1.2	0.2	*	7.5	-2.8	*	-0.9	*	*	*	*	*	0.9	-0.9	3.3	0.2	1.5
Dy	*	-0.1	*	*	1.2	*	*	*	*	*	*	*	*	*	*	*	*	0.5	*	*
Er	*	-0.2	*	*	0.8	*	*	*	*	*	*	*	*	*	*	*	*	0.8	*	*
Eu	*	1.9	*	*	-0.3	*	*	*	*	*	*	*	1.4	*	*	*	*	-4.0	*	*
F	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ga	1.1	0.2	*	*	2.6	*	-0.9	*	-1.4	*	*	-0.9	*	*	*	-0.3	*	1.6	0.2	*
Gd	0.0	0.7	*	*	2.2	*	*	*	*	*	*	*	*	*	*	*	*	0.0	*	*
Ge	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Hf	*	0.9	*	*	0.8	*	*	*	*	*	*	0.9	*	0.3	*	*	*	14.5	*	*
Hg	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ho	*	0.2	*	*	0.5	*	*	*	*	*	*	*	1.9	*	*	*	*	0.1	*	*
I	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
In	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ir	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
La	0.4	0.7	*	*	1.4	*	0.4	*	*	*	*	*	0.3	*	*	*	*	6.6	*	*
Li	0.5	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Lu	*	-0.2	*	*	0.6	*	*	*	*	*	*	*	-1.2	*	*	*	*	*	*	*
Mo	*	-1.2	*	*	*	*	6.9	*	*	*	*	*	*	*	*	*	*	-4.2	*	*
N	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Nb	*	-0.7	*	*	1.2	*	-3.0	-0.7	*	*	*	2.3	*	*	*	*	-0.9	1.9	2.3	-0.3
Nd	*	1.3	*	*	1.5	*	-1.5	*	*	*	*	-1.5	-1.3	*	*	*	4.7	-1.1	*	*
Ni	0.4	*	*	5.6	-0.7	*	*	-0.3	*	*	*	0.0	*	*	*	-4.3	-0.7	5.8	-0.9	0.7
Os	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Pb	*	*	*	-5.2	2.3	*	10.3	-0.3	*	*	*	1.4	*	*	*	-3.0	-0.4	-1.5	-0.9	-0.2
Pd	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Pr	*	0.5	*	*	0.0	*	-1.3	*	*	*	*	*	*	*	*	*	*	4.1	*	*
Pt	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Rb	0.3	*	*	*	-0.5	*	-0.9	-0.3	*	*	*	1.0	*	0.2	*	0.4	0.5	3.3	-1.0	0.4
Re	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Rh	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ru	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
S	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Sb	*	0.2	*	*	9.2	*	*	*	*	*	*	*	-0.2	*	*	*	103.4	*	*	*
Sc	*	*	*	*	*	*	*	*	-1.5	*	*	-0.8	*	0.2	*	*	-0.7	7.8	*	*
Se	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Sm	*	0.3	*	*	-0.4	*	*	*	*	*	*	*	-0.2	*	*	*	*	9.7	*	*
Sn	*	*	*	*	29.4	*	*	*	*	*	*	*	*	*	*	*	*	-5.0	*	*
Sr	1.0	*	*	*	2.5	*	-0.7	-0.3	*	*	0.7	*	*	-1.0	0.0	-0.2	0.5	0.3	0.6	*
Ta	*	-0.1	*	*	0.7	*	*	*	*	*	*	*	*	*	*	*	*	-11.0	*	*
Tb	*	0.3	*	*	0.1	*	*	*	*	*	*	*	1.0	*	*	*	*	33.0	*	*
Te	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Th	1.3	0.2	*	*	0.8	*	*	*	3.4	*	*	*	*	0.2	*	*	*	-2.2	*	-3.2
Tl	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Tm	*	0.3	*	*	0.3	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
U	*	-0.2	*	*	0.5	*	*	*	5.5	*	*	*	*	*	*	*	*	5.4	*	*
V	2.7	*	*	*	5.2	*	*	-0.6	*	-1.1	*	*	*	*	-1.0	2.1	3.2	0.4	0.8	*
W	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Y	0.6	-0.5	*	*	0.8	*	-1.2	1.3	*	*	*	-1.2	*	*	-0.5	-1.7	-3.2	2.2	-0.8	*
Yb	*	0.1	*	*	1.1	*	*	*	*	*	*	*	-0.3	*	*	*	11.8	*	*	*
Zn	0.1	*	*	1.4	7.9	*	0.5	-1.0	*	*	-2.0	*	*	*	0.3	0.1	2.0	0.2	0.6	*
Zr	-0.7	-0.4	*	*	*	-2.8	-0.6	0.6	*	*	-0.7	*	*	*	*	0.5	0.8	4.8	0.1	1.3




Round identifier	P17	P18	P19	P20	P21	P22	P23	P24	P24	P25	P26	P27	P28	P28	P29	P30	P31	P32	P33	P34	
Sample	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	
Technique codes	A.M	M	X	AA.M	X	A	M.X	M	M	X	AAISE	AAA	T.X	X	A.M	AAA	AAA	A.M.X	M	AAA	
Test portion (g)	0.1	0.1	0.7-6	0.1-0.76	0.6-6.4	0.5-1	0.1-5	0.1	0.1	10-10	0.6-10	0.5	0.15-6	6	0.25	0.2-1	0.1-8	0.2-12	0.066	0.1-0.8	
Data quality	2	2	2	1	2	1	2	1	2	2	2	1	1	2	2	2	1	2	1	1	
Technique codes			O.X							T.X					O.M.V	M.X					
SiO2	0.4	*	0.1	0.4	-0.1	-1.6	-0.8	*	*	0.0	-0.6	*	0.7	*	0.7	0.1	0.1	-0.6	*	-0.2	
TiO2	0.0	*	0.0	-0.2	-0.1	-0.9	0.7	*	*	0.1	-3.0	-0.4	-0.8	*	0.7	0.5	0.0	-0.4	*	0.0	
Al2O3	-0.7	*	0.1	-0.2	0.1	0.5	0.3	*	*	0.7	-0.9	5.8	0.6	*	0.9	0.2	-1.1	-0.4	*	0.3	
Fe2O3T	-0.7	*	0.0	0.0	-0.4	4.7	0.3	*	*	0.3	0.1	-3.9	0.6	*	-0.6	1.2	0.3	-0.6	*	-0.5	
Fe(t)O	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
MnO	-0.5	*	0.5	0.8	-0.1	1.0	0.5	*	*	-0.6	-0.7	3.5	0.5	*	0.8	-0.1	-1.2	0.5	*	1.0	
MgO	0.1	*	-0.4	-0.4	-0.5	-1.2	-0.7	*	*	-0.2	-1.6	1.9	1.1	*	-0.1	-0.3	-2.5	-0.7	*	-0.4	
CaO	-0.7	*	-0.3	-0.3	-0.1	3.0	0.4	*	*	0.2	-0.2	3.2	0.1	*	-0.8	-0.9	-1.4	-0.3	*	-0.1	
Na2O	1.7	*	-4.3	1.9	-1.5	6.9	-2.5	*	*	-0.3	-2.6	-0.3	0.8	*	1.0	0.4	-0.8	-0.3	*	-1.9	
K2O	1.9	*	-0.2	3.0	0.5	-11.2	1.1	*	*	0.2	-0.9	-7.8	1.0	*	1.7	0.4	1.3	-0.7	*	-1.5	
P2O5	0.0	*	0.0	6.7	-0.2	-12.6	0.8	*	*	-0.2	1.6	-1.6	1.1	*	0.6	-0.1	-3.5	0.0	*	3.1	
H2O+	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
CO2	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
LOI	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ag	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
As	*	*	*	*	-0.1	584.6	0.8	*	*	2.6	-0.6	*	*	*	*	-0.4	-2.8	-0.6	*	-0.6	
Au	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
B	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ba	0.3	-1.8	*	1.8	0.6	3.7	-0.6	-1.5	*	-1.2	2.2	0.3	-0.7	*	-0.1	0.0	-3.1	0.7	0.0	-0.1	
Be	*	*	*	*	*	-1.8	*	*	*	*	*	*	*	*	0.4	-0.7	*	-0.9	0.4	0.7	*
Bi	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Br	*	*	*	*	*	*	*	*	*	*	2.3	*	*	*	*	*	-1.7	0.2	*	1.1	*
Cd	*	*	*	*	*	*	*	*	*	*	-0.8	*	*	*	*	0.2	35.8	6.3	*	0.0	*
Ce	0.3	-1.1	*	0.3	2.2	-1.5	*	0.5	*	3.1	*	*	*	2.0	-0.7	0.1	3.7	0.2	-0.3	1.1	*
Cl	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Co	-0.1	*	-1.6	-1.6	1.7	22.3	-0.7	*	*	*	0.6	10.4	*	*	-0.8	-0.1	1.9	-0.6	-0.9	0.7	*
Cr	0.6	*	-1.6	-1.4	0.2	1.4	-0.4	*	*	1.0	-1.4	*	0.4	*	-0.2	0.1	2.4	-0.7	-0.9	-0.4	*
Cs	0.2	-0.7	*	-0.2	*	*	*	0.0	*	*	*	*	*	*	-0.5	0.3	*	0.6	1.7	-1.3	*
Cu	-1.3	*	-0.1	-0.2	0.2	5.3	-0.7	*	*	0.1	2.2	0.6	-0.4	*	0.3	0.3	-1.3	-0.5	-0.3	1.0	*
Dy	-0.1	-0.8	*	0.0	*	3.8	*	0.4	*	*	*	*	*	*	-0.4	0.6	1.8	0.1	-0.3	-0.4	*
Er	-0.4	-0.7	*	-0.4	*	6.0	*	0.4	*	*	*	*	*	*	-0.1	0.3	1.8	0.2	-0.8	-0.6	*
Eu	0.3	-0.8	*	0.0	*	-4.0	*	0.3	*	*	*	*	*	*	0.3	0.1	0.6	-0.8	-0.4	1.0	*
F	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ga	*	*	*	0.2	-0.8	*	-1.4	*	*	-0.9	-1.5	*	*	*	-0.6	0.0	-0.6	0.4	0.1	0.3	*
Gd	-0.6	-0.6	*	1.9	*	66.8	*	0.2	*	*	*	*	*	*	-0.7	0.2	*	0.2	-0.7	1.1	*
Ge	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Hf	0.3	0.0	*	-1.2	*	*	0.9	*	-0.3	*	*	*	*	*	0.0	0.1	-5.0	0.7	-2.3	0.6	*
Hg	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ho	-0.1	-0.5	*	0.3	*	*	*	0.3	*	*	*	*	*	*	0.4	-0.1	-0.3	0.1	0.3	0.1	*
I	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
In	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ir	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
La	0.2	-1.3	*	-0.1	2.1	-5.1	*	0.6	*	-1.0	*	*	*	0.4	-2.8	-0.2	3.1	-0.1	-0.3	0.2	*
Li	*	*	*	*	*	*	*	*	*	*	*	0.9	*	*	*	0.0	*	-0.3	*	2.3	*
Lu	-0.4	-0.3	*	0.2	*	*	*	0.3	*	*	*	*	*	*	-0.2	-0.1	1.7	0.0	-1.0	0.7	*
Mo	-1.6	*	*	*	*	*	*	*	0.2	*	*	*	*	*	-3.1	-0.7	-0.6	-0.2	*	-0.3	*
N	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Nb	-0.2	-0.1	*	1.1	1.4	259.9	-1.7	*	0.9	-5.1	0.3	*	-1.2	*	-1.3	0.6	-2.3	-0.3	-1.1	*	*
Nd	0.8	-0.7	*	1.5	0.3	-4.1	*	1.1	*	*	*	*	*	*	-0.2	0.4	0.9	0.8	0.7	1.6	*
Ni	0.7	*	2.9	0.5	-0.9	2.9	*	*	*	1.1	-1.2	-1.4	0.3	*	-1.2	0.0	-2.3	-0.2	0.5	1.4	*
Os	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Pb	*	-0.1	1.4	0.5	-1.2	454.9	-1.3	1.2	*	1.7	-0.5	5.1	0.5	*	*	-0.2	-0.4	-0.3	-2.4	-1.1	*
Pd	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Pr	0.4	-0.8	*	1.2	*	*	*	0.7	*	*	*	*	*	*	-0.9	0.2	2.8	-0.1	0.2	-0.4	*
Pt	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Rb	2.3	0.9	*	0.1	-0.4	9.1	-0.6	0.5	*	-0.2	-0.7	*	0.1	*	-1.0	-0.6	-2.5	-0.8	-0.9	0.3	*
Re	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Rh	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ru	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
S	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Sb	-2.2	*	*	*	*	2647.3	*	*	*	*	*	*	*	*	*	-0.8	*	-1.1	*	8972.7	*
Sc	-0.4	2.8	*	-0.2	0.3	*	*	*	*	1.7	*	5.3	*	*	0.1	0.1	3.1	-0.8	0.2	1.0	*
Se	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Sm	0.2	-1.0	*	0.6	*	0.1	*	0.0	*	*	*	*	*	*	-0.4	-0.1	0.1	0.1	0.2	1.7	*
Sn	0.4	*	*	*	*	5.9	*	*	*	*	*	*	*	*	-1.2	-1.3	0.8	-0.8	*	*	*
Sr	-0.1	1.4	0.3	0.2	0.0	-9.9	-0.8	1.2	*	-0.3	0.0	1.5	-0.2	*	0.6	0.6	-2.6	-0.3	-0.1	0.6	*
Ta	-0.3	-0.4	*	0.5	*	*	*	*	*	*	*	*	*	*	-0.2	2.5	14.9	-0.3	-0.6	1.0	*
Tb	-0.2	-0.7	*	0.4	*	*	*	0.1	*	*	*	*	*	*	-0.4	0.1	0.7	-0.1	-0.1	0.0	*
Te	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Th	-0.2	0.1	5.4	-0.5	*	*	1.1	0.5	*	-7.6	6.4	*	*	-1.1	-0.6	-0.3	2.1	0.8	-0.9	-0.2	*
Tl	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	-0.1	27.3	-1.3	1.4	-0.3	*
Tm	0.1	-0.4	*	0.5	*	*	*	0.0	*	*	*	*	*	*	0.0	-0.1	0.8	-0.1	0.0	0.3	*
U	-0.1	-0.1	*	0.0	*	*	7.3	0.7	*	-6.6	7.3	*	*	2.7	-0.5	-0.1	11.0	1.0	-0.8	0.0	*
V	-0.1	*	0.5	-0.7	0.4	*	-0.7	*	*	-0.7	-4.1	2.4	1.4	*	-0.6	0.0	0.2	-0.4	0.9	1.3	*
W	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Y	0.3	0.3	*	2.1	0.8	-4.7	-0.5	0.4	*	0.1	0.1	*	2.0	*	1.1	-0.5	-0.1	0.4	1.2	1.4	*
Yb	0.1	-0.5	*	0.1	*	6.6	*	-0.1	*	*	*	*	*	*	-0.2	-0.2	0.8	0.1	-0.9	-0.4	*
Zn	-1.7	*	-0.2	-1.6	-0.6	14.5	-1.1	*	*	0.0	-1.5	3.3	0.0	*	0.9	0.3	-1.2	-0.1	*	1.1	*
Zr	0.0	0.7	*	-2.1	0.7	6.6	-0.3	*	-0.2	0.6	-0.2	-0.9	0.5	*	0.3	0.0	-1.6	0.3	-4.5	1.1	*

Round identifier	P35	P36	P37	P37	P38	P39	P40	P41	P42	P43	P44	P45	P46	P46	P47	P48	P49	P50	P51	P52	
Sample	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	
Technique codes	AA	AO	I	I	X	AIR	I	M	AA	X	AAO	X	X	X	MX	A	AO	AA	AA	AA	
Test portion (g)	0.12	0.5	0.2	0.2	0.4-5	0.2-7	0.04	0.1	0.1-1	0.174	0.004-0.6	0.4	1.0-20	20	0.05-4	0.05-0.5	0.003-5	0.2-3	0.1-5	0.1-0.5	
Data quality	2	2	1	2	2	2	2	1	2	1	1	2	1	2	2	2	2	1	2	1	
SiO2	-0.1	0.4	*	*	-0.5	0.5	*	*	8.1	-0.3	-0.6	0.2	-0.4	*	0.3	*	-0.2	1.2	-0.8	0.0	
TiO2	0.0	0.0	1.4	*	0.3	0.8	*	*	-0.9	-0.9	1.9	0.0	-0.4	*	1.2	-0.2	0.3	-3.2	0.0	0.6	
Al2O3	0.9	-2.6	4.4	*	-0.5	0.2	*	*	29.1	-0.7	1.9	0.2	0.3	*	0.2	-0.2	0.4	-0.6	0.3	0.5	
Fe2O3T	0.6	0.8	-0.8	*	0.7	0.3	0.2	*	-14.3	2.7	1.2	0.1	0.5	*	-0.3	-0.4	0.3	-1.4	0.3	0.2	
Fe(II)O	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
MnO	0.5	-3.1	0.8	*	-1.6	-0.2	*	*	-5.6	0.5	-6.3	0.5	1.0	*	-1.8	0.3	-0.1	7.3	-0.7	*	
MgO	0.7	2.9	5.2	*	-0.2	-0.6	*	*	1.8	1.9	1.4	0.7	-1.2	*	0.9	-0.2	-1.3	-2.9	1.5	*	
CaO	1.7	-0.2	-1.0	*	0.6	-0.5	*	*	-23.0	0.3	1.3	-0.3	-0.7	*	0.2	-0.2	0.8	3.0	-1.3	-0.2	
Na2O	-0.2	-6.7	2.2	*	0.2	1.6	-3.1	*	5.6	-6.9	-1.8	-0.1	-0.7	*	0.1	-0.4	0.9	-0.1	-0.6	-42.2	
K2O	0.8	-0.4	1.2	*	-0.2	-0.2	-4.3	*	58.9	-3.3	-7.8	0.8	-1.8	*	1.7	-1.1	1.1	-2.6	0.2	102.8	
P2O5	0.8	*	*	*	0.2	0.7	*	*	*	-3.0	-1.6	0.0	1.5	*	0.5	0.1	0.0	-4.7	0.0	*	
H2O+	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
CO2	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
LOI	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ag	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
As	0.8	*	-0.9	*	-5.0	-3.3	-2.9	*	*	*	*	*	-7.7	*	*	*	0.3	3.0	*	*	
Au	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
B	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ba	0.0	*	-0.3	*	1.2	0.6	0.1	0.0	*	*	*	*	*	0.4	4.2	0.0	0.0	-2.9	*	*	
Be	0.4	*	*	*	*	1.1	*	*	*	*	*	*	*	*	*	*	-0.7	9.1	*	*	
Bi	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Br	*	*	-1.3	*	*	-2.1	-1.2	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Cd	0.7	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ce	0.1	*	1.4	*	*	0.5	0.0	-0.2	*	*	*	*	*	0.8	0.1	*	0.3	-1.0	*	*	
Cl	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Co	-0.8	*	-0.9	*	-1.2	0.5	0.6	*	-2.9	*	*	*	*	3.1	*	*	-0.1	0.4	*	*	
Cr	-0.8	*	3.6	*	-4.4	0.1	-0.6	*	*	*	*	*	*	-3.0	1.0	*	0.4	0.5	*	*	
Cs	0.2	*	-0.5	*	*	0.8	0.6	0.1	*	*	*	*	*	*	*	*	*	*	*	*	*
Cu	0.1	*	*	*	-0.9	1.9	*	*	-1.1	*	*	*	*	-0.6	*	*	*	0.3	0.3	-2.4	*
Dy	0.4	*	1.9	*	*	0.3	*	0.2	*	*	*	*	*	*	*	-0.3	*	-1.2	-1.3	*	1.9
Er	0.5	*	*	*	*	0.3	*	-0.3	*	*	*	*	*	*	-0.2	*	-0.7	-2.0	*	1.6	
Eu	0.1	*	1.0	*	*	0.2	-0.4	-0.2	*	*	*	*	*	*	0.3	*	-0.8	-2.1	*	2.6	
F	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ga	-0.3	*	*	*	-0.9	0.8	*	*	*	*	*	*	0.5	*	*	*	0.0	*	*	2.7	*
Gd	0.1	*	*	*	*	0.7	*	-0.2	*	*	*	*	*	*	0.3	*	-1.3	-0.7	*	2.4	*
Ge	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Hf	0.9	*	1.4	*	*	-0.1	-0.4	-1.3	*	*	*	*	*	*	*	*	-0.3	*	*	-0.4	*
Hg	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ho	0.4	*	*	*	*	0.2	*	0.1	*	*	*	*	*	*	-0.1	*	-0.4	-1.9	*	1.0	*
I	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
In	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ir	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
La	0.1	*	0.7	*	*	0.6	-0.7	-0.7	*	*	*	*	*	1.0	0.0	*	0.4	-2.7	*	1.9	*
Li	0.9	*	*	*	*	*	*	*	*	*	*	*	*	*	*	-0.5	-0.8	-0.5	-2.9	-1.2	*
Lu	0.6	*	1.2	*	*	0.8	0.6	0.0	*	*	*	*	*	*	-0.1	*	-0.5	-0.7	*	0.4	*
Mo	*	*	*	*	*	-0.5	*	*	*	*	*	*	13.9	*	*	*	*	*	*	*	*
N	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Nb	-0.3	*	*	*	-0.3	-0.7	*	0.2	*	*	*	*	4.6	*	1.5	*	0.3	-0.7	*	*	*
Nd	0.2	*	*	-1.0	*	1.4	0.4	0.4	*	*	*	*	*	*	0.2	*	-1.2	-0.6	*	2.4	*
Ni	-1.3	*	*	*	0.0	-0.4	*	*	-1.2	*	*	*	*	0.8	*	*	0.0	-2.7	-5.9	*	*
Os	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Pb	0.6	*	*	*	2.0	0.0	*	0.0	*	*	*	*	2.9	*	-1.1	*	0.6	5.9	*	*	*
Pd	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Pr	0.3	*	*	*	*	0.1	*	-0.2	*	*	*	*	*	*	0.1	*	0.0	3.5	*	2.0	*
Pt	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Rb	0.0	*	3.2	*	-1.6	-0.1	0.8	-0.9	*	*	*	*	1.4	*	-0.1	*	0.0	-2.4	-0.3	-4.4	*
Re	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Rh	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ru	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
S	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Sb	-1.0	*	*	0.9	*	-0.6	0.8	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Sc	-0.3	*	0.6	*	*	-1.8	0.5	*	*	*	*	*	-4.9	*	*	*	-0.3	-2.3	*	*	*
Se	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Sm	-0.1	*	1.6	*	*	-0.1	-0.9	-0.6	*	*	*	*	*	*	0.1	*	-1.4	1.4	*	1.7	*
Sn	-0.4	*	*	*	*	2.1	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Sr	0.2	*	*	0.4	0.8	0.8	*	-0.2	*	*	*	*	0.6	*	0.8	-5.6	0.0	-1.4	-0.9	*	*
Ta	*	*	*	-1.6	*	-2.0	*	-1.1	*	*	*	*	*	*	*	*	*	*	*	*	9.0
Tb	0.3	*	0.2	*	*	0.6	0.3	-0.7	*	*	*	*	*	*	0.0	*	-0.3	*	*	0.1	*
Te	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Th	0.6	*	0.0	*	*	-0.9	0.0	-0.1	*	*	*	*	6.4	*	0.5	*	*	8.6	*	-0.9	*
Tl	0.3	*	*	*	*	-0.3	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Tm	0.4	*	*	*	*	-0.3	*	-0.3	*	*	*	*	*	*	0.0	*	-0.5	-0.2	*	1.1	*
U	0.4	*	*	-0.4	*	0.5	*	-1.0	*	*	*	*	*	*	*	*	*	*	*	0.2	*
V	0.7	*	2.0	*	1.3	1.3	*	*	*	*	*	*	*	-0.6	-2.2	0.3	-0.3	0.6	-2.4	*	*
W	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Y	0.0	*	*	*	*	0.3	*	1.4	*	*	*	*	2.9	*	0.0	*	-0.1	-2.3	*	1.8	*
Yb	0.1	*	0.7	*	*	0.5	0.2	-1.1	*	*	*	*	*	*	-0.2	*	-1.1	0.0	*	1.3	*
Zn	-0.6	*	*	-6.0	-0.7	0.9	*	*	0.5	*	*	*	0.4	*	*	0.3	0.1	0.6	-0.3	3.6	*
Zr	-0.9	*	*	0.6	-0.7	0.6	*	*	*	*	*	*	1.2	*	1.3	-1.0	0.0	-0.1	-9.1	*	*


Round identifier	P52	P53	P54	P55	P56	P57	P58	P59	P60	P61	P62	P63	P64	P65	P66	P67	P68	P69		
Sample	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN		
Technique codes	AAA	MX	X	X	AAIR	AIR	X	X	AX	MX	A,MX	AAA	X	LR	AM	AM	AAA	AAA	AAA	
M					TX							M,OX			OX	OX				
Test portion (g)	0.1-0.5	0.1-10	1.5	5	0.1-1	0.2-4	5	1	9	1-1.5	0.2-3.5	0.2-1	0.06-5	1	0.1-1.4	0.05-4	0.05-4	0.1	1.0-3	0.1-5
Data quality	2	1	2	2	1	2	2	1	2	2	1	2	2	1	1	2	2	2	2	2
SiO2	*	0.4	-0.4	*	0.1	-0.6	3.3	0.3	*	0.2	-0.8	1.1	-1.0	-2.9	*	1.1	*	-0.2	0.4	-0.5
TiO2	*	-0.6	-0.2	*	-0.9	0.5	-1.4	-0.7	*	-0.2	-1.0	-0.2	-0.3	1.0	*	0.5	*	2.8	0.7	0.4
Al2O3	*	0.4	-0.7	*	0.0	0.6	-3.5	0.1	*	0.1	0.0	-0.7	-0.6	-3.4	0.9	0.0	*	-0.5	0.2	0.2
Fe2O3T	*	-0.3	-1.9	*	-0.5	0.6	-2.3	0.3	*	-0.2	3.7	-1.2	7.2	-4.8	-4.2	0.9	*	0.2	1.0	-0.7
Fe(II)O	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
MnO	0.0	-0.4	0.3	*	1.0	0.5	-1.9	-0.7	*	0.5	0.1	0.5	-0.3	-3.8	1.0	-1.4	*	1.2	0.5	-0.3
MgO	0.0	1.3	-0.4	*	-0.7	-0.2	-8.2	3.1	*	0.0	2.1	-5.4	1.7	0.3	*	-0.7	*	-0.4	-0.7	-0.8
CaO	*	0.3	-0.9	*	-0.2	2.1	-8.8	-0.2	*	0.1	0.5	-0.2	0.9	-0.3	*	0.2	*	-0.2	0.4	0.3
Na2O	*	0.0	-0.7	*	0.7	1.2	-5.8	0.6	*	1.0	0.8	-0.2	-3.0	18.8	1.6	1.2	*	0.2	-2.4	-0.1
K2O	*	-1.1	-0.7	*	-1.1	0.4	-2.2	0.4	*	0.4	0.6	1.0	-1.3	-0.3	-7.4	0.4	*	-0.2	0.4	-0.4
P2O5	-0.4	2.6	0.6	*	0.0	-0.8	-7.1	0.0	*	0.0	0.8	0.0	-0.7	-6.3	*	-1.6	*	*	-0.8	0.5
H2O+	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
CO2	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
LOI	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Aq	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
As	3.0	-1.0	*	*	*	*	*	*	*	-1.5	*	0.0	*	*	0.2	*	-0.4	*	-1.5	-8.4
Au	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
B	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ba	1.2	-1.1	*	*	-0.8	-0.2	*	*	-1.3	-3.9	0.6	-0.7	1.1	0.5	-0.7	*	0.4	0.0	-1.8	1.5
Be	6.6	-0.1	*	*	-0.1	*	*	*	*	*	*	*	4.0	*	*	-0.6	*	-0.2	*	*
Bi	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Br	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Cd	1.7	-0.2	*	*	-2.4	*	*	*	*	*	*	-0.8	*	*	*	*	3.6	*	4.6	*
Ce	*	-0.4	*	*	-0.3	*	*	*	*	*	-0.3	0.5	-1.5	*	*	-1.1	0.6	-0.6	*	*
Cl	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Co	2.3	0.6	*	*	-0.6	-0.7	*	*	*	*	-1.6	0.8	0.2	-0.1	*	0.2	*	1.1	-0.3	
Cr	1.8	0.4	*	*	3.9	1.4	*	*	-3.5	0.4	-0.3	-0.7	-1.7	-0.8	*	-0.9	0.5	-3.5	-2.4	
Cs	*	0.6	*	*	0.3	*	*	*	*	0.3	-0.2	-0.9	*	-1.3	*	-0.4	*	-0.2	*	*
Cu	2.6	0.3	*	-0.9	-0.6	-0.4	*	-0.6	*	-1.0	-0.6	1.3	*	*	*	0.1	0.0	-0.9	0.3	
Dy	*	0.3	*	*	-0.2	*	*	*	*	1.4	0.6	-1.1	*	0.2	*	-0.6	*	-1.7	*	*
Er	*	0.3	*	*	-0.1	*	*	*	*	0.4	0.5	-1.4	*	*	*	-0.2	*	-2.2	*	*
Eu	*	0.7	*	*	-0.3	*	*	*	*	1.0	0.5	-1.1	*	0.3	*	0.3	*	-0.6	*	*
F	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ga	*	0.2	*	*	-0.6	-0.2	*	-0.5	*	0.9	-5.6	4.5	0.5	*	*	-0.3	0.9	1.7	*	*
Gd	*	0.4	*	*	-0.1	*	*	*	*	0.6	0.5	-1.7	*	*	*	-0.5	*	-1.3	*	*
Ge	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Hf	*	-0.3	*	*	6.1	0.1	*	*	*	-2.0	-0.1	-3.1	*	0.5	*	-0.7	*	-2.1	*	*
Hg	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ho	*	0.3	*	*	-0.2	*	*	*	*	1.1	0.4	-1.0	*	*	*	-0.3	*	-1.8	*	*
I	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
In	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ir	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
La	*	-0.3	*	*	-0.5	*	*	*	*	0.9	0.2	0.2	*	0.1	*	-1.2	1.6	-1.9	*	*
Li	*	1.5	*	*	0.5	*	*	*	*	*	0.1	4.5	*	*	*	-0.7	0.5	2.0	-4.2	*
Lu	*	-0.2	*	*	-0.2	*	*	*	*	0.3	0.2	-1.3	*	0.9	*	-0.2	*	-1.4	*	*
Mo	3.8	0.1	*	*	0.9	*	*	*	*	*	*	*	*	*	*	0.2	*	0.6	*	*
N	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Nb	1.7	1.7	*	2.3	7.2	-0.2	*	0.7	*	0.3	-1.6	2.7	*	*	*	-0.3	*	4.9	*	*
Nd	*	0.9	*	*	0.2	*	*	*	*	-0.2	1.0	-1.0	*	-0.2	*	-0.4	*	-0.8	*	*
Ni	3.5	0.0	*	1.5	-1.4	0.1	*	2.8	-1.4	0.7	0.7	2.7	-0.7	*	*	0.1	1.0	-1.1	-0.7	*
Os	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Pb	-0.5	0.5	*	0.9	-4.8	0.3	*	1.9	*	-0.1	-0.6	0.5	*	*	*	-0.3	*	4.8	*	*
Pd	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Pr	*	0.2	*	*	-0.1	*	*	*	*	-0.7	0.7	-0.9	*	*	*	-0.7	*	-1.3	*	*
Pt	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Rb	*	0.0	*	0.4	-0.6	-0.2	*	2.1	*	0.9	-0.4	1.4	2.7	0.3	*	1.1	*	-1.0	*	*
Re	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Rh	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Ru	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
S	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Sb	29.9	-1.8	*	*	*	*	*	*	*	*	-2.3	*	*	-0.5	*	0.7	*	-1.0	*	*
Sc	8.1	0.5	*	-4.6	-0.7	-0.4	*	*	*	1.9	-0.4	2.2	0.2	-0.3	*	-1.6	*	-1.4	*	*
Se	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Sm	*	0.5	*	*	-0.4	*	*	*	*	0.7	0.8	-0.7	*	0.3	*	-0.5	*	-0.9	*	*
Sn	3.1	0.3	*	3.8	-0.8	*	*	*	*	-2.0	-0.7	*	*	*	*	0.0	*	0.0	*	*
Sr	1.0	-0.1	*	0.0	0.5	0.0	*	-1.1	*	2.9	-0.4	1.6	*	*	*	-0.9	0.0	-2.0	-0.9	*
Ta	*	-1.9	*	*	0.7	*	*	*	*	0.8	*	1.0	*	1.4	*	-1.3	*	7.5	*	*
Tb	*	0.4	*	*	-0.3	*	*	*	*	0.8	0.3	-1.2	*	0.2	*	-0.6	*	-1.5	*	*
Te	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Th	*	0.3	*	*	-2.2	0.1	*	6.0	*	-1.1	-0.5	-2.5	*	1.2	*	-0.6	*	-1.1	*	*
Tl	*	-0.5	*	*	0.3	*	*	*	*	*	*	*	*	*	*	-0.8	*	0.5	*	*
Tm	*	0.6	*	*	0.0	*	*	*	*	0.3	0.4	-1.2	*	*	*	-0.3	*	-1.5	*	*
U	*	-0.4	*	2.7	5.4	0.3	*	*	*	-0.5	-0.6	-2.1	*	0.7	*	-0.9	*	0.4	*	*
V	4.6	0.6	*	*	-0.3	0.0	*	0.8	-1.6	-0.7	0.4	1.0	-2.2	*	*	-0.3	0.2	-2.7	-0.6	*
W	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*	*
Y	*	0.8	*	1.1	-0.9	-0.5	*	-0.8	*	6.0	0.0	0.5	-2.4	*	*	-0.8	1.0	-3.9	-1.2	*
Yb	*	-0.2	*	*	-0.2	*	*	*	*	-0.4	0.4	-1.0	*	1168.2	*	-0.2	*	-2.5	*	*
Zn	*	0.2	*	0.1	-0.4	-1.4	*	-0.9	0.3	-3.7	-2.3	0.8	*	*	*	0.2	1.5	0.6	-0.5	*
Zr	0.0	0.7	*	1.2	1.2	0.1	*	0.5	*	-4.0	0.5	0.2	-2.6	*	*	1.1	2.0	-3.3	-1.9	*

Round identifier	P70	P71	P72	P73	P74	P74	P75	P76	P77	P78
Sample	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN	MSAN
Technique codes	X	A,M,X	X	M	R,M	X	X	M	I	X
Test portion (g)	1.0-6	0.2-0.5	0.6	0.25	0.04-7.5	7.5	5	0.1	0.1	0.1-0.27
Data quality	2	1	1	1	1	2	2	1	2	1
SiO2	0.2	0.1	1.5	*	-0.5	*	-0.4	*	*	0.6
TiO2	-22.5	0.3	-1.2	*	0.7	*	0.3	*	*	0.6
Al2O3	1.2	-0.2	0.1	*	0.5	*	-1.7	*	*	0.8
Fe2O3T	0.2	0.4	-1.7	*	0.8	*	6.3	*	-0.5	1.1
Fe(II)O	*	*	*	*	*	*	*	*	*	*
MnO	-0.2	*	-1.2	*	0.1	*	-0.8	-1.4	*	2.5
MgO	-0.3	-0.4	-1.5	*	-0.4	*	*	*	*	0.4
CaO	-0.2	0.0	0.4	*	0.5	*	*	*	*	0.9
Na2O	1.2	-1.0	0.2	*	0.9	*	*	*	*	0.5
K2O	-0.2	0.6	-0.6	*	-1.1	*	-3.0	*	*	-0.3
P2O5	0.8	0.8	0.6	*	1.4	*	*	*	*	2.3
H2O+	*	*	*	*	*	*	*	*	*	*
CO2	*	*	*	*	*	*	*	*	*	*
LOI	*	*	*	*	*	*	*	*	*	*
Ag	*	*	*	*	*	*	*	*	*	*
As	1.9	*	*	*	*	*	*	*	*	2.7
Au	*	*	*	*	*	*	*	*	*	*
B	*	*	*	*	*	*	*	*	*	*
Ba	1.3	-2.3	*	-1.0	0.6	*	*	0.5	*	-1.5
Be	*	-3.5	*	*	*	*	*	-0.7	*	-0.3
Bi	*	*	*	*	*	*	*	*	*	*
Br	-1.0	*	*	*	*	*	*	*	*	*
Cd	172.1	*	*	*	*	*	*	6.4	*	-1.7
Ce	-0.4	-0.4	*	-1.4	-2.8	*	*	0.5	*	-2.7
Cl	*	*	*	*	*	*	*	*	*	*
Co	-2.4	2.2	*	-0.9	-1.5	*	*	-0.4	-0.6	*
Cr	-1.6	2.6	*	*	3.0	*	*	-0.2	*	2.0
Cs	*	*	*	3.0	*	*	*	0.5	0.4	-1.3
Cu	-1.1	-3.0	*	-0.4	0.6	*	*	-0.4	*	4.1
Dy	*	-1.4	*	1.2	-1.9	*	*	0.1	*	0.0
Er	*	0.4	*	0.7	-1.6	*	*	0.7	*	0.5
Eu	*	-0.6	*	1.0	-0.2	*	*	0.3	0.1	1.4
F	*	*	*	*	*	*	*	*	*	*
Ga	-0.9	*	*	9.3	0.5	*	*	1.1	*	0.6
Gd	*	0.1	*	0.1	-1.6	*	*	-1.3	*	0.1
Ge	*	*	*	*	*	*	*	*	*	*
Hf	5.1	*	*	0.0	-1.1	*	*	0.0	-0.2	-1.2
Hg	*	*	*	*	*	*	*	*	*	*
Ho	*	0.0	*	-0.8	-1.0	*	*	0.3	*	0.1
I	*	*	*	*	*	*	*	*	*	*
In	*	*	*	*	*	*	*	*	*	*
Ir	*	*	*	*	*	*	*	*	*	*
La	0.4	-0.2	*	-1.4	-2.3	*	*	0.4	0.1	-0.8
Li	*	-6.2	*	*	*	*	*	0.2	*	*
Lu	*	*	*	1.4	-1.0	*	*	0.5	-0.6	0.4
Mo	6.9	*	*	*	*	*	*	-0.1	*	1.2
N	*	*	*	*	*	*	*	*	*	*
Nb	3.6	*	*	-1.3	-1.8	*	*	-0.9	*	0.1
Nd	*	-0.6	*	-0.3	-1.6	*	*	1.4	-1.4	0.0
Ni	-1.4	-2.1	*	*	2.2	*	*	0.5	*	0.8
Os	*	*	*	*	*	*	*	*	*	*
Pb	-0.2	3.1	*	*	-0.3	*	*	0.8	*	1.8
Pd	*	*	*	*	*	*	*	*	*	*
Pr	*	-0.1	*	-1.0	-1.6	*	*	0.7	*	-0.4
Rb	0.0	*	*	-2.9	-1.2	*	*	-0.9	0.6	0.1
Re	*	*	*	*	*	*	*	*	*	*
Rh	*	*	*	*	*	*	*	*	*	*
Ru	*	*	*	*	*	*	*	*	*	*
S	*	*	*	*	*	*	*	*	*	*
Sb	*	*	*	*	*	*	*	0.0	*	34.6
Sc	*	*	*	*	-4.2	*	*	2.0	-0.1	1.0
Se	*	*	*	*	*	*	*	*	*	*
Sm	*	0.5	*	-0.8	-1.3	*	*	-0.2	-0.2	1.4
Sn	*	*	*	*	*	*	*	*	*	-5.0
Sr	-0.7	-1.8	*	-0.9	0.0	*	*	0.2	*	1.2
Ta	*	*	*	1.4	-2.4	*	*	0.4	*	-8.4
Tb	*	*	*	2.0	-1.4	*	*	-0.5	-0.1	*
Te	*	*	*	*	*	*	*	*	*	*
Th	*	0.0	*	-0.7	-1.3	*	*	0.0	0.1	3.8
Tl	*	*	*	*	*	*	*	-0.4	*	*
Tm	*	*	*	-0.1	-0.8	*	*	0.3	*	*
U	*	-0.1	*	-0.2	-1.9	*	*	0.4	-0.1	0.7
V	-4.8	-2.7	*	-1.2	-0.1	*	*	*	*	-0.1
W	*	*	*	*	*	*	*	*	*	*
Y	0.7	-2.3	*	-1.8	-1.1	*	*	-0.1	*	5.6
Yb	*	-0.4	*	-0.6	-1.4	*	*	0.3	0.2	1.1
Zn	-0.9	-2.6	*	*	-0.2	*	*	2.2	*	1.7
Zr	1.4	*	*	-2.2	-0.5	*	*	0.1	*	-0.9


GeoPT15 - Barchart for SiO<sub>2</sub>




GeoPT15 - Barchart for TiO<sub>2</sub>




GeoPT15 - Barchart for Al<sub>2</sub>O<sub>3</sub>




GeoPT15 - Barchart for Fe<sub>2</sub>O<sub>3</sub>




GeoPT15 - Barchart for MnO



GeoPT15 - Barchart for MgO



GeoPT15 - Barchart for CaO



GeoPT15 - Barchart for Na<sub>2</sub>O





Figure 1 (Part 1). GeoPT15 — MSAN ocean floor sediment: Data distribution charts for elements for which values were assi Horizontal lines show the limits for  $-2 < z < 2$  for pure geochemistry labs (solid lines) and  $-2 < z' < 2$  for applied geochemistry labs (pecked lines).

GeoPT15 - Barchart for K2O



GeoPT15 - Barchart for P2O5






Figure 1 (Part 1). GeoPT15 — MSAN ocean floor sediment: Data distribution charts for elements for which values were assigned. Horizontal lines show the limits for  $-2 < z < 2$  for pure geochemistry labs (solid lines) and  $-2 < z' < 2$  for applied geochemistry labs (pecked lines).


GeoPT15 - Barchart for Fe(II)O



GeoPT15 - Barchart for CO2

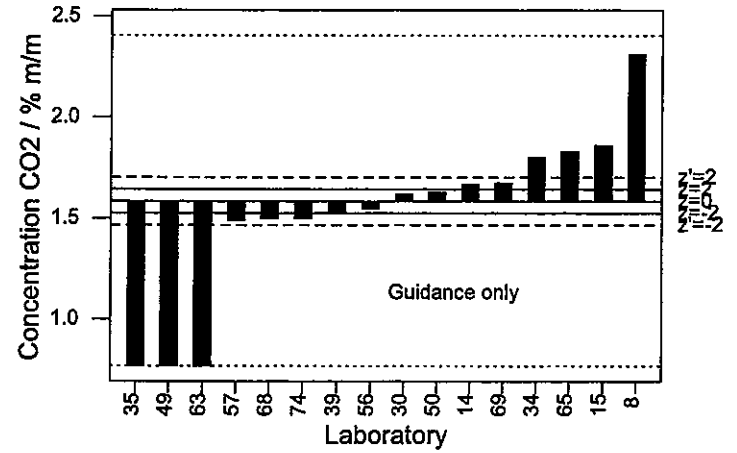

GeoPT15 - Barchart for H2O+



GeoPT15 - Barchart for LOI


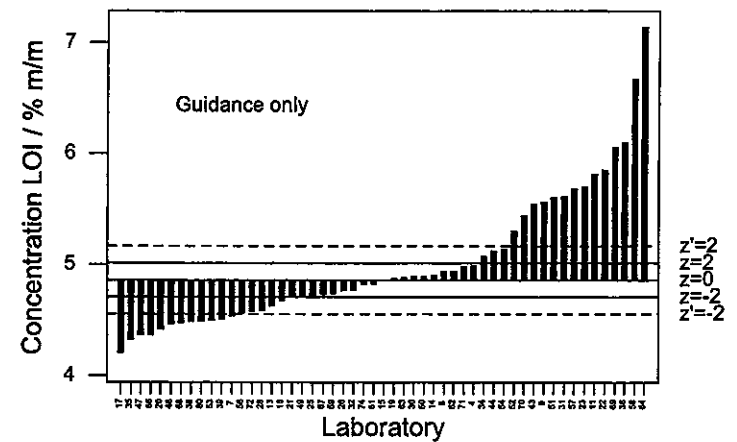



Figure 2 (Part 1). GeoPT15 — MSAN ocean floor sediment: Data distribution charts for elements for which only guidance values can be given or where no value could be assigned.




GeoPT15 - Barchart for Cs




GeoPT15 - Barchart for Cu




GeoPT15 - Barchart for Dy




GeoPT15 - Barchart for Er




GeoPT15 - Barchart for Eu



GeoPT15 - Barchart for Ga



GeoPT15 - Barchart for Gd



GeoPT15 - Barchart for Hf




Figure 1 (Part 2). GeoPT15 — MSAN ocean floor sediment: Data distribution charts for elements for which values were assigned. Horizontal lines show the limits for  $-2 < z < 2$  for pure geochemistry labs (solid lines) and  $-2 < z' < 2$  for applied geochemistry labs (pecked lines).





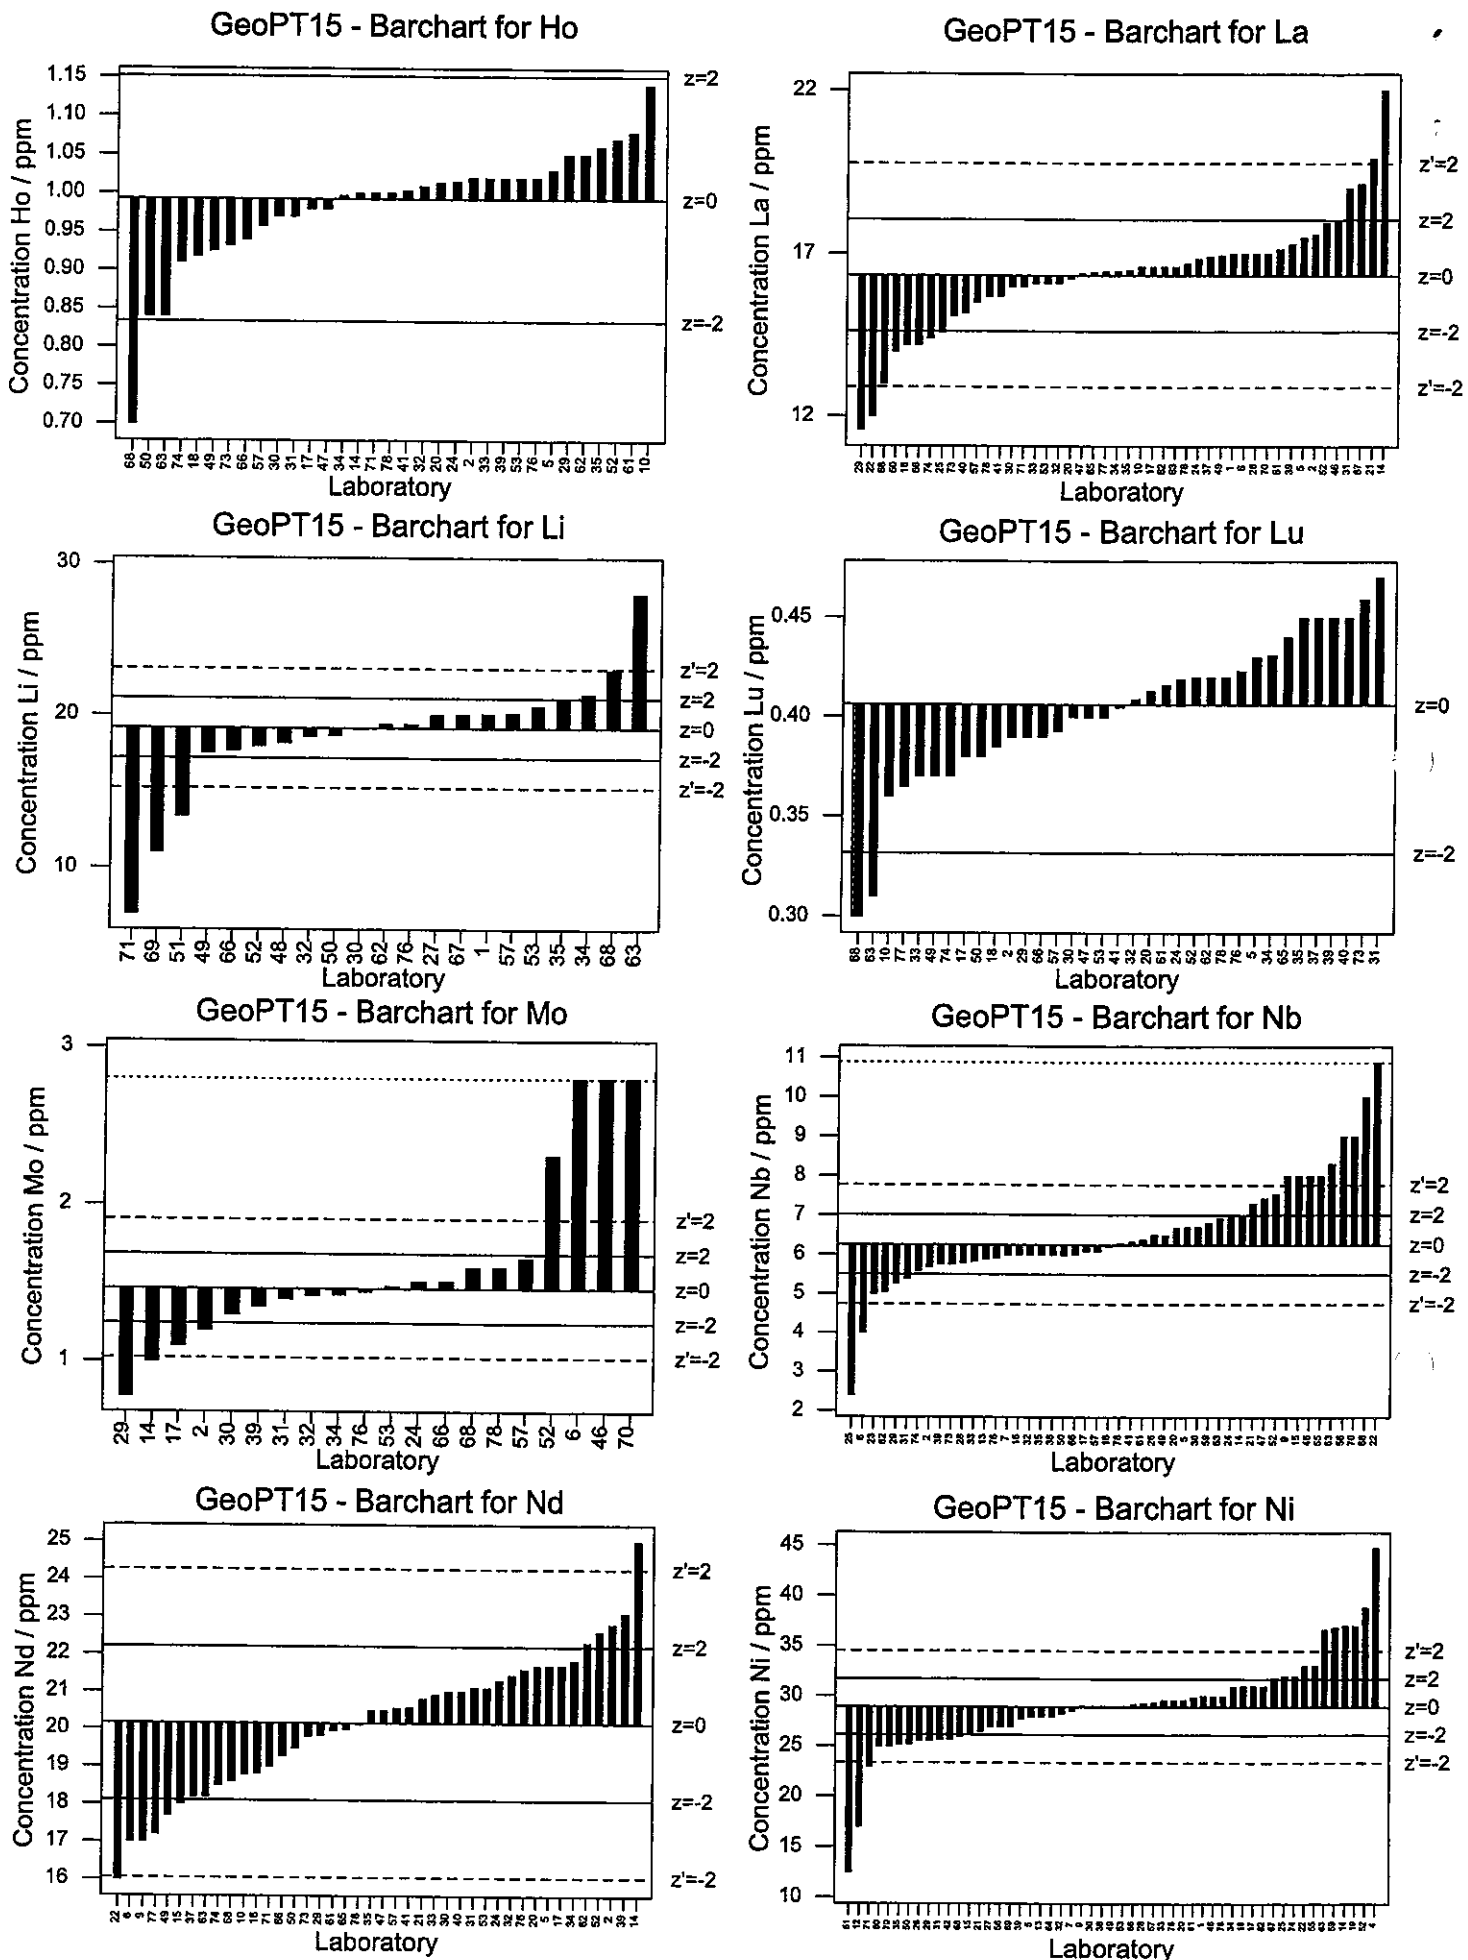


Figure 1 (Part 2). GeoPT15 — MSAN ocean floor sediment: Data distribution charts for elements for which values were assigned. Horizontal lines show the limits for  $-2 < z < 2$  for pure geochemistry labs (solid lines) and  $-2 < z < 2$  for applied geochemistry labs (pecked lines).


GeoPT15 - Barchart for Pb




GeoPT15 - Barchart for Pr




GeoPT15 - Barchart for Rb




GeoPT15 - Barchart for Sb




GeoPT15 - Barchart for Sc



GeoPT15 - Barchart for Sm



GeoPT15 - Barchart for Sn



GeoPT15 - Barchart for Sr






Figure 1 (Part 2). GeoPT15 — MSAN ocean floor sediment: Data distribution charts for elements for which values were assigned. Horizontal lines show the limits for  $-2 < z < 2$  for pure geochemistry labs (solid lines) and  $-2 < z' < 2$  for applied geochemistry labs (pecked lines).


GeoPT15 - Barchart for Ta




GeoPT15 - Barchart for Tb




GeoPT15 - Barchart for Th




GeoPT15 - Barchart for Tl




GeoPT15 - Barchart for Tm



GeoPT15 - Barchart for U



GeoPT15 - Barchart for V



GeoPT15 - Barchart for Y






Figure 1 (Part 2). GeoPT15 — MSAN ocean floor sediment: Data distribution charts for elements for which values were assigned. Horizontal lines show the limits for  $-2 < z < 2$  for pure geochemistry labs (solid lines) and  $-2 < z' < 2$  for applied geochemistry labs (pecked lines).

GeoPT15 - Barchart for Yb



GeoPT15 - Barchart for Zn



GeoPT15 - Barchart for Zr





Figure 1 (Part 2). GeoPT15 — MSAN ocean floor sediment: Data distribution charts for elements for which values were assigned. Horizontal lines show the limits for  $-2 < z < 2$  for pure geochemistry labs (solid lines) and  $-2 < z' < 2$  for applied geochemistry labs (pecked lines).

GeoPT15 - Barchart for Se



GeoPT15 - Barchart for W



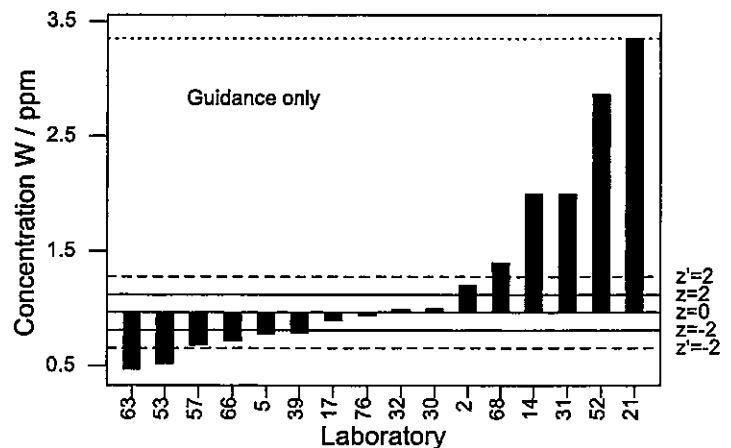


Figure 2 (Part 2). GeoPT15 — MSAN ocean floor sediment: Data distribution charts for elements for which only guidance values can be given or where no value could be assigned.


GeoPT15 - Barchart for B




GeoPT15 - Barchart for Bi




GeoPT15 - Barchart for Cl




GeoPT15 - Barchart for F




GeoPT15 - Barchart for Ge



GeoPT15 - Barchart for Hg



GeoPT15 - Barchart for I



GeoPT15 - Barchart for S




Figure 2 (Part 2). GeoPT14 — MSAN ocean floor sediment: Data distribution charts for elements for which only guidance values can be given or where no value could be assigned.

# Multiple z-score chart – GeoPT15

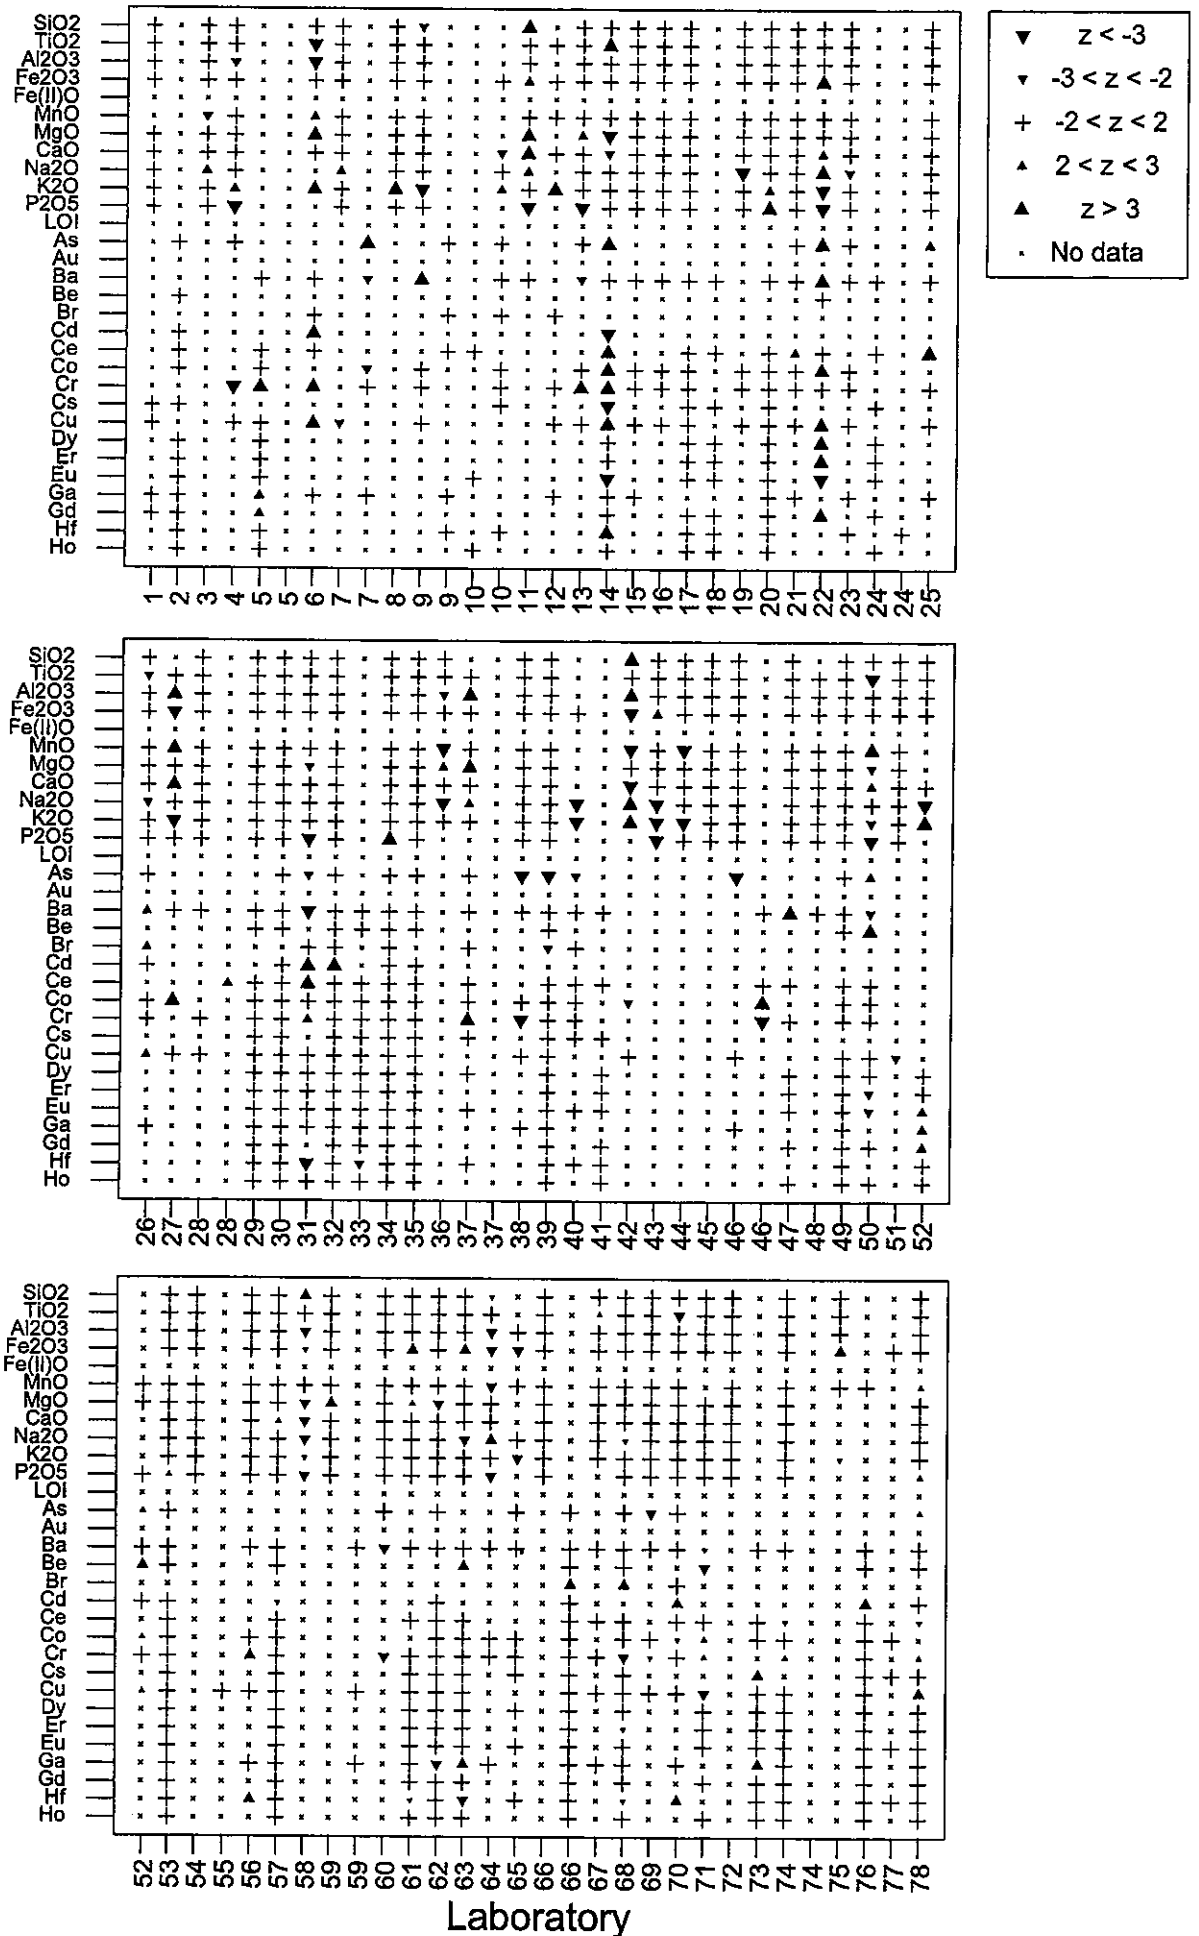


Figure 3 (Part 1) GeoPT15 — MSAN ocean floor sediment: Multiple z-score charts for laboratories participating in the GeoPT15 round. Symbols indicate whether or not an elemental result complies with the  $-2 < z < +2$  criteria. Satisfactory data are plotted as '+'. Data for other categories are plotted as follows:  $z < -3$  (▼),  $-3 < z < -2$  (▼),  $+2 < z < +3$  (▲),  $z > +3$  (▲).

